



OIML Member State

The Netherlands



Number R117/2019-A-NL1-22.10 revision 2 Project number 3619036 Page 1 of 7

Issuing authority Person responsible: NMi Certin B.V. M.Ph.D. Schmidt



Applicant and Manufacturer

Endress+Hauser Flowtec AG

Kägenstrasse 7 4153 Reinach **Switzerland**

Identification of the certified type

A measurement transducer

Type: Promass F 300 DNx^[1]; Promass F 500 DNx^[1]; Promass O 300 DNx^[1]; Promass O 500 DNx^[1]; Promass X 300 DNx^[1]; Promass X 500 DNx^[1]; Promass Q 300 DNx^[1]; Promass Q 500 DNx^[1];

Characteristics

See page 2 and further.

This OIML Certificate is issued under scheme A

This Certificate attests the conformity of the above-identified type (represented by the sample(s) identified in the OIML Type Evaluation Report) with the requirements of the following Recommendation of the International Organization of Legal Metrology (OIML):

R 117-1:2019 "Dynamic measuring systems for liquids other than water"

Accuracy class 0.3 / 0.5 / 1.0 / 1.5

This Certificate relates only to the metrological and technical characteristics of the type of measuring instrument covered by the relevant OIML International Recommendation identified above. This Certificate does not bestow any form of legal international approval.


This certificate and supporting reports comply with the requirements of OIML-CS-PD-07 clause 6.2.

Important note: Apart from the mention of the Certificate's reference number and the name of the OIML Member State in which the Certificate was issued, partial quotation of the Certificate and of the associated OIML Type Evaluation Report(s) is not permitted, although either may be reproduced in full.

With x denoting the size of the meter (diameter of the in- and outlet in mm).

Issuing Authority

NMi Certin B.V., OIML Issuing Authority NL1 15 March 2024



This document is issued under the provision that no liability is accepted and that the applicant shall indemnify third-party liability.

The notification of NMi Certin B.V. as Issuing Authority can be verified at www.oiml.org

This document is digitally signed and sealed. The digital signature can be verified in the blue ribbon at the top of the electronic version of this certificate.







NMi Certin B.V. Thijsseweg 11 2629 JA Delft The Netherlands T +31 88 636 2332 certin@nmi.nl www.nmi.nl





OIML Member State The Netherlands



Number R117/2019-A-NL1-22.10 revision 2 Project number 3619036 Page 2 of 7

OIML Certificate

The conformity was established by the results of tests and examinations provided in the associated reports:

Report number	Issue date	Number of pages
NMi-2466149-03	2 January 2023	63
N	Measurement sensor: Pro	mass F
PF/6491	2 July 1996	77
CVN-302404-01 rev. 1	27 June 2003	15
CPC-407631-1	31 March 2005	42
CPC-412432-1	31 March 2005	32
CPC-10200667-1	9 August 2010	7
NMi-10201056-1	29 March 2012	6
NMi-12200688-01	3 December 2013	6
NMi-14200053-01	16 April 2014	6
NMi-15200446-01	22 June 2016	5
NMi-1902055-01	31 August 2018	11
NMi-2389303-02	12 February 2021	11
NMi-2463103-01	12 February 2021	11
NMi-3147081-01	8 September 2022	16
NMi-3619040-01	15 March 2024	15
NMi-3619045-01	15 March 2024	13
N	leasurement sensor: Pro	mass O
NMi-12200149-1	24 May 2012	6
N	leasurement sensor: Pro	mass Q
NMi-15200323-01a	12 February 2021	11
NMi-1901704-01	31 August 2018	10
NMi-2389303-01	12 May 2020	29
NMi-2389303-03	12 February 2021	10
NMi-2466149-01	12 August 2022	56
NMi-3147081-01	8 September 2022	16
N	leasurement sensor: Pro	mass X
NMi-11200539-01	2 April 2012	6
	Promass 300/500 electro	onics
NMi-16200475-01a	2 January 2023	31
NMi-1901185-01	1 November 2017	35
NMi-2202829-01	3 December 2019	40
NMi-3619036-01	15 March 2024	12









OIML Member StateThe Netherlands



Number R117/2019-A-NL1-22.10 revision 2 Project number 3619036 Page 3 of 7

Characteristics of the measurement transducer



In Tables 1 to 6, the general characteristics of the measuring instrument are presented. The construction of the measurement transducer is recorded in documentation folders TC7149-8 for the measurement sensor and TC10822-4 for the electronics.

Table 1 General characteristics applicable to all Promass measurement sensors

- Density range: 300 ... 1400 kg/m³ for mass measurement

400 ... 1400 kg/m³ for volume and density measurement

- Maximum viscosity: 1000 mPa·s

Accuracy class:
 Environmental classes:
 Ambient temperature range:
 0.3; 0.5; 1.0 and 1.5
 M3 / E2 + E3^[2] / H3
 -40 ... +55 °C

- Intended for the measurement of: Oil and oil products, chemicals, potable liquids, liquefied gases

under pressure measured at temperatures above -10 °C, liquified gases under pressure measured below -10 °C, liquefied carbon dioxide and liquefied natural gas (LNG

including vapour return measurement).

Sensor Type ^[3]	Oil and oil products, chemicals, and potable liquids	Liquefied gases under pressure	Liquefied gases below -10 °C, cryogenic liquids, LNG, LCO ₂	
		Accuracy class		
	0.3; 0.5	1.0	1.5	
Promass F	MDV	MDV	M	
Promass O	MDV	-	M	
Promass X	MDV	MDV	M	
Promass Q	MDV	MDV	M	







^[2] Environmental class E3 only applicable in combination with DC-DC convertor and an OIML R117:2019 approved flow computer which is also certified for class E3.



^[3] This table indicates the approved measurements: **M** for Mass, **D** for density, and **V** for volume.





OIML Member State The Netherlands



Number R117/2019-A-NL1-22.10 revision 2 Project number 3619036 Page 4 of 7

Table 2 Specific characteristics of the Promass F measurement sensors

Sensor size	DN8	DN15	DN25	DN40	DN50	
Maximum flow rate [kg/min]	30	100	300	700	1000	
Minimum flow rate [kg/min][4]	1,5	5	15	37,5	58,3	
Minimum flow rate [kg/min] ^[5]	0,75	2,5	7,5	18,75	29,15	
Minimum Measured Quantity [kg]	2	5	20	20	20	

Sensor size	DN80	DN100	DN150	DN250	
Maximum flow rate [t/h]	180	270	720	2200	
Minimum flow rate [t/h] ^[4]	9	14	32	90	
Minimum flow rate [t/h] ^[5]	4,5	7	16	45	
Minimum Measured Quantity [kg]	200	200	500	1000	


Further characteristics of the Promass F:

Accuracy Class	0.3	0.5	1.0	1.5		
Maximum pressure 🕂	100 bar(g)					
Temperature range liquid for mass measurement	-	-10 °C +200 °C				
Temperature range liquid for density and volume measurement		-10 °C +90 °C				









^[5] For accuracy class 1.0 and 1.5





OIML Member StateThe Netherlands



Number R117/2019-A-NL1-22.10 revision 2 Project number 3619036 Page 5 of 7

Table 3 Specific characteristics of the Promass O measurement sensors



Sensor size	DN80	DN100	DN150	DN250	
Maximum flow rate [t/h]	180	270	720	2200	
Minimum flow rate [t/h] ^[6]	9	14	32	90	
Minimum flow rate [t/h] ^[7]	4,5	7	16	45	
Minimum Measured Quantity [kg]	200	200	500	1000	


Further characteristics of the Promass O:

Accuracy Class	0.3	0.5	1.0	1.5
Maximum pressure		oar(g)		
Temperature range liquid for mass measurement	-10 °C	+200 °C	NA	-40 °C +90 °C ^[8]
Temperature range liquid for density and volume measurement	-10 °C +90 °C		NA	NA

Table 4 Specific characteristics of the Promass X measurement sensors

Sensor size	DN350						
Maximum flow rate [t/h]	3353						
Minimum flow rate [t/h] ^[9]	137						
Minimum flow rate [t/h] ^[10]	68,5						
Minimum Measured Quantity [kg]	1000						

Further characteristics of the Promass X:

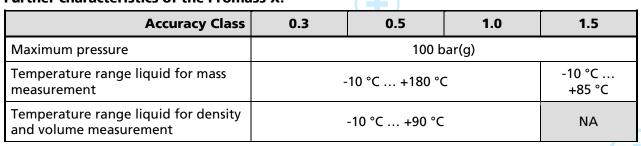



[7] For accuracy class 1.0 and 1.5

[8] Product temperature range for measuring liquefied CO₂ (LCO₂)

[9] For accuracy class 0.3 and 0.5

[10] For accuracy class 1.0 and 1.5







OIML Member State The Netherlands



Number R117/2019-A-NL1-22.10 revision 2 Project number 3619036 Page 6 of 7

OIML Certificate

Table 5 Specific characteristics of the Promass Q measurement sensors



Sensor size	DN25	DN50	DN80	DN100	DN150	DN200
Maximum flow rate [t/h]	20	80	200	400	850	1500
Minimum flow rate [t/h] ^[11]	0,45	2	6	14	16	24
Minimum flow rate [t/h] ^[12]	0,225	1	3	7	8	12
Minimum Measured Quantity [kg]	10	20	100	200	200	200

Sensor size	DN250			
Maximum flow rate [t/h]	2400			
Minimum flow rate [t/h] ^[11]	50			
Minimum flow rate [t/h] ^[12]	25			
Minimum Measured Quantity [kg]	500			


Further characteristics of the Promass Q:

Accuracy Class	0.3	0.5	1.0	1.5	
Maximum pressure 🕕	100 bar(g)				
Temperature range liquid for mass measurement	-	-200 °C +90 °C			
Temperature range liquid for density and volume measurement	-	NA			









[12] For accuracy class 1.0 and 1.5





OIML Member StateThe Netherlands



Number R117/2019-A-NL1-22.10 revision 2 Project number 3619036 Page 7 of 7

OIML Certificate

Table 6 General characteristics of the Promass 300 and Promass 500 electronics

Environmental classes	M3 / E2 + E3 ^[13] / H3	
Ambient temperature range	-40+55 °C; condensing humidity	
Power supply voltage	24 VDC 100240 VAC, 5060 Hz 24 VDC / 100240 VAC, 5060 Hz	

Software identification

Version number	Checksum		Version	Checksum	
	Modbus	Hart	number	Modbus	Hart
01.00.02[14]	0xE87F	0x321F	01.02.00	0x5645	-
01.00.03 ^[14]	0x79B5	0x1585	01.02.01	0x559B	-
01.00.04	0xE109	0xB075	01.02.02	0x0A92	-
01.01.01	0xA476	0x977D	01.02.03	0xECE3	-
01.01.02	0x2AAB	0xED44	01.05.00	0xA9EE	0xB4A1
01.01.03	0x6A37	0x86FC	01.05.01	0x2B95	0x59D4
01.01.04	0x6D79	0x674	01.05.02	0xF1B7-	0xE6B5
01.01.05	0x4670-	0x559B	01.05.03	-	0xD79D
01.01.06	-	0x0891	01.06.00	0x8894	0x4BDD
01.01.07	-	0xB7B2	01.06.01	0x58FD	0x9BB4

The Promass 300 and Promass 500 flow transmitters may only be used in combination with Coriolis measurement sensors manufactured by Endress+Hauser Flowtec AG.

Certificate history

Revision	Date	Description of the modification
0	2 January 2023	Initial release.
1	30 May 2023	Addition of software version 01.06.01.
2	15 March 2024	Addition of: - Environmental class E3 - Liquid CO ₂ applications for Promass O - Minimum density lowered for mass measurements.

^[13] Environmental class E3 only applicable in combination with DC-DC convertor and an OIML R117:2019 approved flow computer which is also certified for class E3.



^[14] This software version is only allowed for the Promass 300 electronics.