
Automatic level gauges for measuring the level
of liquid in stationary storage tanks

Part 3: Report format for type evaluation

Jaugeurs automatiques pour le mesurage des niveaux de liquide
dans les réservoirs de stockage fixes

Partie 3: Format de rapport pour l'examen de type



Contents

Foreword4

1 Introduction 5

2 Applicability of this Report Format 5

3 Guidance for the application of this Report Format 5

4 Evaluation Report..... 5

Foreword

The International Organization of Legal Metrology (OIML) is a worldwide, intergovernmental organization whose primary aim is to harmonize the regulations and metrological controls applied by the national metrological services, or related organizations, of its Member States. The main categories of OIML publications are:

- **International Recommendations (OIML R)**, which are model regulations that establish the metrological characteristics required of certain measuring instruments and which specify methods and equipment for checking their conformity. OIML Member States shall implement these Recommendations to the greatest possible extent;
- **International Documents (OIML D)**, which are informative in nature and which are intended to harmonize and improve work in the field of legal metrology;
- **International Guides (OIML G)**, which are also informative in nature and which are intended to give guidelines for the application of certain requirements to legal metrology; and
- **International Basic Publications (OIML B)**, which define the operating rules of the various OIML structures and systems.

OIML Draft Recommendations, Documents and Guides are developed by Technical Committees or Subcommittees which comprise representatives from the Member States. Certain international and regional institutions also participate on a consultation basis. Cooperative agreements have been established between the OIML and certain institutions, such as ISO and the IEC, with the objective of avoiding contradictory requirements. Consequently, manufacturers and users of measuring instruments, test laboratories, etc. may simultaneously apply OIML publications and those of other institutions.

International Recommendations, Documents, Guides and Basic Publications are published in English (E) and translated into French (F) and are subject to periodic revision.

Additionally, the OIML publishes or participates in the publication of **Vocabularies (OIML V)** and periodically commissions legal metrology experts to write **Expert Reports (OIML E)**. Expert Reports are intended to provide information and advice, and are written solely from the viewpoint of their author, without the involvement of a Technical Committee or Subcommittee, nor that of the CIML. Thus, they do not necessarily represent the views of the OIML.

This publication - reference OIML R 85-3, edition 2008 (E) - was developed by the OIML Technical Subcommittee TC 8/SC 1 *Static volume and mass measurement*. It was approved for final publication by the International Committee of Legal Metrology in 2008. Together with R 85-1 & 2, edition 2008 (E), this edition supersedes the previous edition of OIML R 85 (Edition 1998).

OIML Publications may be downloaded from the OIML web site in the form of PDF files. Additional information on OIML Publications may be obtained from the Organization's headquarters:

Bureau International de Métrologie Légale
11, rue Turgot - 75009 Paris - France
Telephone: 33 (0)1 48 78 12 82
Fax: 33 (0)1 42 82 17 27
E-mail: biml@oiml.org
Internet: www.oiml.org

Automatic level gauges for measuring the level of liquid in fixed storage tanks

Part 3: Report Format for type evaluation

1 Introduction

This Report Format applies for any kind of electric or electronic level gauge (independent of its technology), but with the exclusion of purely mechanical level gauges. It presents a standardized format for the results of the various tests and examinations, described in Part 2 of this Recommendation, to which a type of an automatic level gauge shall be submitted with a view to its approval based on International Recommendation OIML R 85 (2008).

It is recommended that all metrology services or laboratories evaluating and/or testing types of automatic level gauges according to OIML R 85 or to national or regional regulations based on OIML R 85 use this Report Format, directly or after translation into a language other than English or French. In case of a translation, it is highly recommended to leave the structure and the numbers of the clauses unchanged: in this case most of the contents is also understandable for those who can not read the language of the translation.

It is also recommended that this Report Format in English or in French (or in both languages) be transmitted by the country performing the tests to the relevant authorities of another country, under bi- or multi-lateral cooperation agreements.

In the practical application of the Report Format, in addition to a cover page by the Issuing Authority, as a minimum clauses A–F (as necessary) shall be included.

2 Applicability of this Report Format

In the framework of the OIML Certificate System for Measuring Instruments, and the OIML Mutual Acceptance Arrangement (MAA) applicable to automatic level gauges in conformity with OIML R 85, the use of this Report Format is mandatory.

Implementation of this Report Format is informative with regard to the implementation of OIML R 85-1 & 2 Part 1 in national regulations.

3 Guidance for the application of this Report Format

In case a prescribed test is not relevant for the type of instrument to be tested, the reason why the test is omitted shall be clearly stated in the field “Remarks” (for instance tests related to AC mains supply in the case of an instrument powered by DC mains) or partial testing after modification of a previously tested type.

The number of the report and the page numbers shall be completed in the heading.

The user is free to change the length of the cells (for instance “Remarks”) as required in a specific case.

4 Evaluation Report

The format for the Evaluation Report is given on the following pages.

Cover page by the Issuing Authority

Contents of the Evaluation Report

A	Authority responsible for this report	8
B	Synopsis of the results of the examinations and tests	8
C	Summary of the results of the examination and tests	9
	C.1 Examinations	9
	C.2 Performance tests	9
D	General information	10
	D.1 Manufacturer	10
	D.2 Applicant	10
	D.3 Testing laboratories involved in the tests	11
	D.4 General information concerning the type	12
	D.5 Accessories supplied by the applicant	12
	D.6 Selection of sample(s) tested	13
	D.7 Adjustments and modifications	14
	D.8 Choice of the manufacturer concerning the severity levels	14
	D.9 Full details about the electrical power requirements	15
	D.10 Additional information concerning the type	15
	D.11 Documentation supplied by the applicant	16
	D.12 Information concerning the test equipment used for the type evaluation	17
E	Examination	18
	E.1 Constituents (4)	18
	E.2 Units of measurement (5)	18
	E.3 Rated operating conditions (6.1)	19
	E.4 Special conditions (6.1)	19
	E.5 Indicating device (7.1)	19
	E.6 Printer(s) (7.1.9)	20
	E.7 Movable sensor (7.2)	20
	E.8 Installation (7.3)	21
	E.9 Ancillary devices (7.4)	21
	E.10 Markings (7.5)	22
	E.11 Verification marks (7.6)	22
	E.12 Mechanical sealing (7.7)	23
	E.13 Electronic sealing (7.7)	23
	E.14 Safeguarding the integrity of the measurement (7.8)	24
F	Performance tests	25
	F.1 Accuracy (8.1.5.2)	25
	F.2 Discrimination (8.1.5.3)	27
	F.3 Hysteresis (8.1.5.4)	28
	F.4 Influence factor tests	29
	F.4.1 Static environmental temperatures (8.1.6.2)	29
	F.4.2 Mains voltage variations (8.1.6.3 and 8.1.6.4)	31
	F.5 Disturbance tests	32
	F.5.1 Damp heat, cyclic (condensing) (8.1.7.1)	32
	F.5.2 Radiated, radio-frequency, electromagnetic fields (8.1.7.2.1)	33
	F.5.3 Conducted, radio-frequency, electromagnetic fields (8.1.7.2.2)	34
	F.5.4 Electrostatic discharge (8.1.7.2.3)	35
	F.5.5 Bursts on signal, data and control lines (8.1.7.2.4)	36
	F.5.6 Surges on signal, data and control lines (8.1.7.2.5)	37
	F.5.7 AC mains voltage dips, short interruptions and voltage variations (8.1.7.2.6)	38
	F.5.8 Bursts (transients) on AC and DC mains (8.1.7.2.7)	39
	F.5.9 Voltage dips, short interruptions and voltage variations on DC mains power (8.1.7.2.8)	40
	F.5.10 Ripple on DC mains power (8.1.7.2.9)	41
	F.5.11 Surges on AC and DC mains power lines (8.1.7.2.10)	42

A Authority responsible for this report

Name	
Address	
Report number	
Application number	
Date/period of tests	
Date of issuing this Report	
Name and signature of the responsible person	
Stamp(s) (if applicable)	

B Synopsis of the results of the examinations and tests*(To be completed by the Issuing Authority)*

The tested specimen fulfils ALL the applicable requirements in OIML R 85 (2008)	YES	NO
Remarks:		

C Summary of the results of the examination and tests

(To be completed by the Issuing Authority)

C.1 Examinations

For details, refer to the examination: Clause E of this report as indicated in the first column.

Sub-clause	Test (with reference to requirement in Part 1)	+	-	Remarks	Page
E.1	Constituents (4)				
E.2	Units of measurement (5)				
E.3	Rated operating conditions (6.1)				
E.4	Special conditions (6.1)				
E.5	Indicating device (7.1)				
E.6	Printer(s) (7.1.9)				
E.7	Movable sensor (7.2)				
E.8	Installation (7.3)				
E.9	Ancillary devices (7.4)				
E.10	Markings (7.5)				
E.11	Verification marks (7.6)				
E.12	Mechanical sealing (7.7)				
E.13	Electronic sealing (7.7)				
E.14	Safeguarding the integrity of the measurement (7.8)				

C.2 Performance tests

For details, refer to the tests: clause F in this report as indicated in the first column.

F.1	Accuracy (8.1.5.2)				
F.2	Discrimination (8.1.5.3)				
F.3	Hysteresis (8.1.5.4)				
F.4.1	Temperature tests (8.1.6.2)				
F.4.2	Mains voltage variations (8.1.6.3 + 8.1.6.4)				
F.5.1	Damp heat, cyclic (condensing) (8.1.7.1)				
F.5.2	Radiated, radio-frequency, electromagnetic fields (8.1.7.2.1)				
F.5.3	Conducted, radio-frequency, electromagnetic fields (8.1.7.2.2)				
F.5.4	Electrostatic discharge (8.1.7.2.3)				
F.5.5	Bursts on signal, data and control lines (8.1.7.2.4)				
F.5.6	Surges on signal, data and control lines (8.1.7.2.5)				
F.5.7	AC mains voltage dips, short interruptions and voltage variations (8.1.7.2.6)				
F.5.8	Bursts (transients) on AC and DC mains (8.1.7.2.7)				
F.5.9	Voltage dips, short interruptions and voltage variations on DC mains power (8.1.7.2.8)				
F.5.10	Ripple on DC mains power (8.1.7.2.9)				
F.5.11	Surges on AC and DC mains power lines (8.1.7.2.10)				

D General information**D.1 Manufacturer**

Company	
Address	

D.2 Applicant

Company	
Representative	
Address	
Reference	
Date of application	

Remarks:

D.3 Testing laboratories involved in the tests*(This table to be completed for each testing laboratory)*

Name	
Address	
Application number	
Tests by this laboratory	
Date/period of tests	
Name(s) of test engineer(s)	
Accredited by	
Accreditation includes R 85	<input type="checkbox"/> Yes <input type="checkbox"/> No
Details of relevant peer assessment or assessment by other means	
In case tests were performed at another location than the premises of this laboratory, give details here	
Name of the responsible person	
Date of signature	
Stamp (if applicable) and signature of the responsible person	

Remarks:

**D.4 General information concerning the type and the sample(s) submitted for the tests
(as stated on the instrument / provided by the manufacturer).**

Manufacturer's trade mark / corporate name		
Year of manufacture		
Type designation		
Model number (if applicable)		
Serial number(s) of the sample(s)		
Measuring range(s)		
Electrical power		
Identification of software	Version number	
	Checksum/identification code	
Remarks:		

D.5 Accessories supplied by the applicant

Operating instructions	
Data printer	
Cables	
Ancillary facilities	
Power supply unit	
Other accessories / remarks:	

D.6 Selection of sample(s) tested

In case the tests and examination are valid for more versions, give full details of the types, versions, measuring ranges, etc.:

Justification for the selection of the samples:

D.7 Adjustments and modifications

Adjustments, modifications, and repairs made to the samples during the testing:

D.8 Choice of the manufacturer concerning the severity levels

Influence	Severity level
Dry heat	(1, 2, 3, 4):
Cold	(1, 2, 3, 4):
DC mains voltage variation	High level: Low level:

D.9 Full details about the electrical power requirements

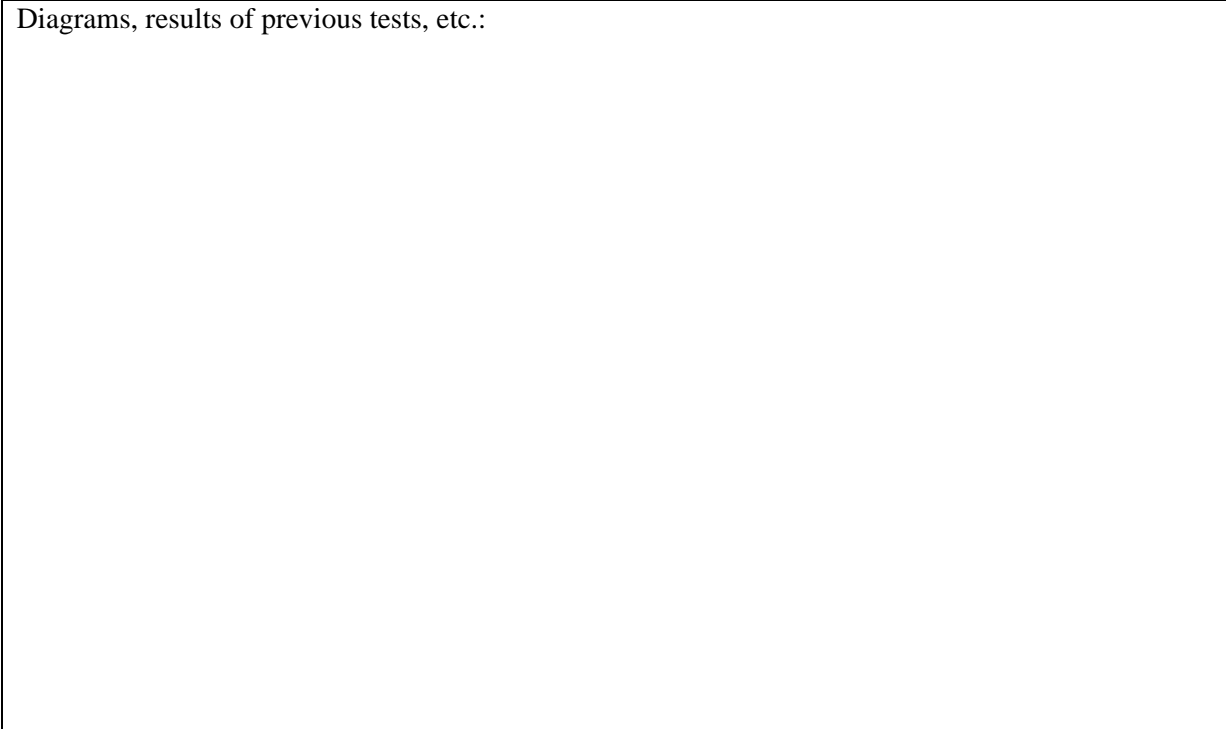
--

D.10 Additional information concerning the type

Additional remarks and/or information (connection equipment, interfaces, etc.):
Remarks:

D.11 Documentation supplied by the applicant

Diagrams, results of previous tests, etc.:

A large empty rectangular box with a thin black border, intended for the applicant to provide diagrams, test results, or other documentation. The box is currently blank.

D.12 Information concerning the test equipment used for the type evaluation

(including details of simulations)

If applicable, the laboratory is free to provide this information, instead of a complete overview here, in the appropriate chapter F.x in an extra field below the 1st table (with “Date”, etc.).

In this case, a statement shall be made in this field.

E Examination

(to be completed by the Examining authority)

E.1 Constituents (4)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

Liquid level sensor	
Transducer	
Correction sensor	
Calculator	
Indicating device(s)	
Printer	
Ancillary devices	
Checking facilities	
Others	
Remarks:	

E.2 Units of measurement (5)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

	Display	Print
Dip		
Ullage		
Other indication(s)		
Remarks:		

E.3 Rated operating conditions (6.1)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

Temperature extreme values	Liquid	
	Medium above liquid	
Pressure extreme values		
Liquid characteristics		
Liquid density extreme values		
Medium characteristics		
Medium density extreme values		
Remarks:		

E.4 Special conditions (6.1)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

Remarks:	

E.5 Indicating device (7.1)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

Subclause	Requirement	Remarks	+	-
7.1.1	Distance between analog scale marks			
7.1.2	Number of indicating devices			
7.1.3	Common indicating device			
7.1.4	Remote indication duly identified			
7.1.2-3-4	Other indicating devices			
7.1.2	Alarm when outside limits			
7.1.5	Default display of dip / ullage			
7.1.6	Display of measurement			
7.1.7	Symbol or name of unit present			
	Scale interval			
7.1.8	Digital display			
Remarks:				

E.6 Printer(s) (7.1.9)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

Subclause	Requirement	Remarks	+	-
7.1.2	Number of printers			
7.1.4	Printer duly identified to ALG			
7.1.5	Default print of dip/ullage			
7.1.6	Print of measurement			
7.1.7	Symbol or name of unit present			
	Scale interval			
Remarks:				

E.7 Movable sensor (7.2)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

Subclause	Requirement	Remarks	+	-
7.2.1	Suspension mechanism			
7.2.2	Static position			
Remarks:				

E.8 Installation (7.3)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

Subclause	Requirement	Remarks	+	-
7.3.1.1	Accessible and legible			
7.2.1.2	Verification possible			
7.3.1.3	Gauge hatch			
7.3.1.3	No obstacles			
7.3.1.4	Affect ALG measurement			
7.3.1.5	Influence eddies, etc.			
7.3.1.6	Compensation movement tank			
7.3.1.7	Location correction sensor(s)			
7.3.1.8	Thermal expansion			
Remarks:				

E.9 Ancillary devices (7.4)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

Description	Remarks	+	-
Remarks:			

E.10 Markings (7.5)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

Requirement	Remarks	+	-
Location of the markings			
Name of the manufacturer / trademark			
Type designation			
Serial number			
Year of manufacture			
Type approval mark (provisions)			
Ranges defining the field of operation			
Visibility			
Additional information (if required)			
Remarks:			

E.11 Verification marks (7.6)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

	Remarks	+	-
Location			
Fit for easy application			
Impossible to remove without damage			
Remarks:			

E.12 Mechanical sealing (7.7)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

	Remarks	+	-
Data plate			
Other components			
Impossible to remove without damage			
Remarks:			

E.13 Electronic sealing (7.7)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

	Remarks	+	-
Access			
Password changeable			
Configuration mode			
Event counter			
Date of change parameter			
Value of parameter			
Identification authorized person			
Traceability last intervention			
Remarks:			

E.14 Safeguarding the integrity of the measurement (7.8)

Date:	Observer:	Serial number:
--------------	------------------	-----------------------

Sub-clause	Requirement	Remarks			+ -	
					+	-
7.8.1	Possibility of testing checking facility					
	Checking facility type I or P					
7.8.2.1	Checking facility disturbances	YES	NO			
7.8.2.3	Durability protection facility	YES	NO			
7.8.2.5	Action by checking facility					
7.8.3.1	Protection of data					
7.8.3.2	Integrity of permanent stored instructions					
7.8.3.3	Transfer/storage of data					
7.8.3.4	Checking facility calculator					
7.8.3.5	Checking facility indicating device					
7.8.3.6	Checking facility ancillary device					
Remarks:						

F Performance tests

F.1 Accuracy (8.1.5.2)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

Observations in mm: upwards					
Level	Indication	Error	MPE	+	-

Remarks:

Observations in mm: downwards					
Level	Indication	Error	MPE	+	-

Remarks:

F.2 Discrimination (8.1.5.3)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

Discrimination	Level	Indication	Level change	Indication change	+	-
Upwards						
Downwards						

Remarks:

In the case of an ALG without a movable liquid level detecting element, this test can be skipped.
In this case, this justification shall be mentioned here.

F.3 Hysteresis (8.1.5.4)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

Upwards	Level 1	Level 2	Level 3	Maximum hysteresis	MPE	+	-
Level up							
Indication							
Level down							
Indication							
Hysteresis							

Downwards	Level 1	Level 2	Level 3	Maximum hysteresis	MPE	+	-
Level down							
Indication							
Level up							
Indication							
Hysteresis							

Remarks:

In the case of an ALG without a movable liquid level detecting element, this test can be skipped.
In this case, this justification shall be mentioned here.

F.4 Influence factor tests**F.4.1 Static environmental temperatures (8.1.6.2)**

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Relative humidity	%	%
Atmospheric pressure	hPa	hPa

F.4.1.1 Dry heat (8.1.6.2.1)							
Temperature		Level	Indication	Error	MPE	+	-
Reference temperature	°C						
High temperature	°C						
Reference temperature	°C						

F.4.1.2 Cold (8.1.6.2.2)							
Temperature		Level	Indication	Error	MPE	+	-
Reference temperature	°C						
Low temperature	°C						
Reference temperature	°C						
Remarks:							

F.4.2 Mains voltage variations (8.1.6.3 and 8.1.6.4)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

DC mains voltage variation (8.1.6.3)

AC main voltage variation (8.1.6.4)

Voltage		Level	Indication	Error	MPE	+	-
Reference voltage	V						
High voltage	V						
Low voltage	V						
Reference voltage	V						

Remarks:

F.5 Disturbance tests**F.5.1 Damp heat, cyclic (condensing) (8.1.7.1)**

Observer:	Serial number:
------------------	-----------------------

Test conditions	Begin	End
Date		
Time		
Atmospheric pressure	hPa	hPa

Cycle no.	Time	Low temp. °C	Humidity % RH	Time	High temp. °C	Humidity % RH
1						
2						

Level	Indication	Error	MPE	Action checking facility	+	-

Remarks:

F.5.2 Radiated, radio-frequency, electromagnetic fields (8.1.7.2.1)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

EM field		Level	Indication	Error	MPE	Action checking facility	+	-
Frequency	Field strength							
MHz	V/m							
MHz	V/m							
MHz	V/m							
MHz	V/m							
MHz	V/m							

Remarks:

F.5.3 Conducted, radio-frequency, electromagnetic fields (8.1.7.2.2)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

Field injected on port(s):	
----------------------------	--

EM field		Level	Indication	Error	MPE	Action Checking facility	+	-
Frequency	Amplitude							
MHz	V							
MHz	V							
MHz	V							
MHz	V							
MHz	V							
Remarks:								

F.5.4 Electrostatic discharge (8.1.7.2.3)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

<input type="checkbox"/> Contact discharge	<input type="checkbox"/> Direct application	Test voltage	<input type="text" value="kV"/>
<input type="checkbox"/> Air discharge	<input type="checkbox"/> Indirect application	Number of discharges:	<input type="text"/>

Discharge applied on	Level	Indication	Error	MPE	Action Checking facility		
						+	-

Remarks:

F.5.5 Bursts on signal, data and control lines (8.1.7.2.4)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

Test voltage	kV
--------------	----

Repetition rate	kHz
-----------------	-----

Burst applied on	Polarity +/-	Exposure time	Level	Indication	Error	MPE	Action Checking facility		
								+	-

Remarks:

F.5.6 Surges on signal, data and control lines (8.1.7.2.5)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

Surge applied on	Voltage and polarity	Number of surges	Level	Indication	Error	MPE	Action checking facility	+	-

Remarks:

F.5.7 AC mains voltage dips, short interruptions and voltage variations (8.1.7.2.6)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

Mains voltage and frequency	V	Hz
-----------------------------	---	----

Test	Reduction to	Duration [cycles]	Level	Indication	Error	MPE	Action checking facility	+	-
Dips a	V								
	%								
Dips b	V								
	%								
Dips c	V								
	%								
Dips d	V								
	%								
Dips e	V								
	%								
Short interruption	V								
	%								

Remarks:

F.5.8 Bursts (transients) on AC and DC mains (8.1.7.2.7)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

Test voltage	kV
--------------	----

Repetition rate	kHz
-----------------	-----

Polarity +/-	Exposure time	Level	Indication	Error	MPE	Action checking facility	Action	
							+	-

Remarks:

F.5.9 Voltage dips, short interruptions and voltage variations on DC mains (8.1.7.2.8)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

Test	Reduction to	Duration	Level	Indication	Error	MPE	Action checking facility	+	-
Voltage dips	40 %	0.1 s							
	70 %	0.1 s							
Short interruption	0 %	0.01 s							
Voltage variations	85 %	10 s							
	120 %	10 s							

Remarks:

F.5.11 Surges on AC and DC mains power lines (8.1.7.2.10)

Date of test:	Observer:	Serial number:
----------------------	------------------	-----------------------

Test conditions	Begin	End
Time		
Environmental temperature	°C	°C
Relative humidity	% RH	% RH
Atmospheric pressure	hPa	hPa

	Angle	Voltage and polarity	Number of surges	Level	Indication	Error	MPE	Action checking facility	+	-
Line to line	0°									
	90°									
	180°									
Line to earth	0°									
	90°									
	180°									
270°										

Remarks:

