

ORGANISATION INTERNATIONALE
DE MÉTROLOGIE LÉGALE



INTERNATIONAL RECOMMENDATION

Testing procedures and test report format
for pattern evaluation of fuel dispensers
for motor vehicles

Procédures d'essai et format du rapport d'essai
des modèles de distributeurs de carburant pour véhicules à moteur

OIML R 118

Edition 1995 (E)

R 118 was superseded by R 117-2-2014

CONTENTS

Foreword	3
1 Scope	4
2 Test equipment and test conditions	4
3 Testing procedures	5
3.1 Determination of flowrate	6
3.2 Accuracy	6
3.3 Minimum measured quantity	8
3.4 Flow interruption	8
3.5 Gas elimination device	9
3.6 Variation in the internal volume of hoses	10
3.7 Endurance test	11
4 Additional testing procedures for electronic dispensers	11
4.1 Dry heat (non condensing)	12
4.2 Cold	13
4.3 Damp heat, cyclic (condensing)	13
4.4 Power voltage variations	14
4.5 Short-time power reductions	15
4.6 Electrical bursts	16
4.7 Electrostatic discharges	17
4.8 Electromagnetic susceptibility	18
Annex A Test report format	23
General information concerning the pattern	24
Check list	25
Conclusion of tests	31
Test report	32

FOREWORD

The International Organization of Legal Metrology (OIML) is a worldwide, intergovernmental organization whose primary aim is to harmonize the regulations and metrological controls applied by the national metrological services, or related organizations, of its Member States.

The two main categories of OIML publications are:

- 1) **International Recommendations (OIML R)**, which are model regulations that establish the metrological characteristics required of certain measuring instruments and which specify methods and equipment for checking their conformity; the OIML Member States shall implement these Recommendations to the greatest possible extent;
- 2) **International Documents (OIML D)**, which are informative in nature and intended to improve the work of the metrological services.

OIML Draft Recommendations and Documents are developed by technical committees or subcommittees which are formed by the Member States. Certain international and regional institutions also participate on a consultation basis.

Cooperative agreements are established between OIML and certain institutions, such as ISO and IEC, with the objective of avoiding contradictory requirements; consequently, manufacturers and users of measuring instruments, test laboratories, etc. may apply simultaneously OIML publications and those of other institutions.

International Recommendations and International Documents are published in French (F) and English (E) and are subject to periodic revision.

OIML publications may be obtained from the Organization's headquarters:

Bureau International de Métrologie Légale
11, rue Turgot - 75009 Paris - France
Telephone: 33 (1) 48 78 12 82 and 42 85 27 11
Fax: 33 (1) 42 82 17 27

*
* *

This publication - reference OIML R 118, edition 1995 (E) - was developed within the OIML subcommittee TC 8/SC 3 *Dynamic volume measurement (liquids other than water)*. It was approved for final publication by the International Committee of Legal Metrology in 1994 and will be submitted to the International Conference of Legal Metrology in 1996 for formal sanction.

TESTING PROCEDURES AND TEST REPORT FORMAT FOR PATTERN EXAMINATION OF FUEL DISPENSERS FOR MOTOR VEHICLES

1 Scope

This International Recommendation concerns the metrological controls to which fuel dispensers for motor vehicles shall be submitted in order to verify that their characteristics comply with the requirements of the International Recommendation OIML R 117 *Measuring systems for liquids other than water*. It does not apply to dispensers for liquefied petroleum gases (LPG). The procedures are intended for testing complete systems. For systems where some of the components have been previously approved, the number of tests may be reduced.

The purpose of this Recommendation is to facilitate the recognition of test results among countries. In this way, duplication of tests can be avoided, thereby simplifying considerably the work associated with pattern approval.

The standardized test report format for pattern evaluation of fuel dispensers for motor vehicles is given in Annex A.

2 Test equipment and test conditions

Ambient temperature: except when otherwise specified, the ambient temperature shall not vary by more than 10 °C during the test. Ambient temperature shall be measured close to the dispenser and test equipment. Maximum difference in temperature between ambient and liquid is 10 °C. Liquid temperature shall be measured in the test measure.

Relative humidity: except when otherwise specified, between 30 % and 80 %, and 60 % \pm 15 % on performance tests for electronic dispensers.

Atmospheric pressure: between 86 kPa and 106 kPa.

Mains power voltage: nominal voltage.

Mains power frequency: nominal frequency.

Test liquid: two alternatives, in order of preference:

- 1) test a dispenser with a liquid with which it is intended to be used.
- 2) test a dispenser with a suitable liquid having a viscosity similar to that of the liquid with which the dispenser is intended to be used.

For a dispenser intended to measure liquids with different characteristics, especially diesel and gasoline, tests shall, if appropriate, be performed for each category of product.

Test equipment: shall be designed to permit the dispenser to work within its flowrate and pressure range.

Volume of the supply tank: shall be of sufficient capacity to not cause foaming of the liquid or a rise in temperature during the performance tests.

Standard test measures and their use: shall be in accordance with the International Recommendation OIML R 120 *Standard capacity measures for testing of measuring systems for liquids other than water*.

Preliminary runs: every time the dispenser is connected hydraulically, it shall be operated at the maximum flowrate for at least five minutes before measurement starts. Every time a new work session starts (for example after a stop of one hour or more), the dispenser shall work at the maximum flowrate for at least one minute before measurement starts.

3 Testing procedures

Symbols, units and equations:

P_u	Unit price (price/L)
t	Time (s)
Q	Flowrate of liquid (L/min)
V_i	Volume indication of dispenser (L)
P_i	Price indication (or printed if not fitted with a price indicator) of dispenser (price)
P_c	Calculated price (price)
V_n	Volume indication of test measure or computed volume from simulated pulses (L)
T	Temperature of liquid in the test measure (°C)
T_r	Reference temperature of test measure (°C)
T_m	Temperature of liquid passing through the meter (°C)
E_v	Error of volume indication (%)
E_p	Error of price indication (price)
Q_a	Flowrate of air (L/min)
V_a	Volume of air (L)
α	Cubic expansion coefficient of test liquid due to temperature (°C ⁻¹)
β	Cubic expansion coefficient of test measure due to temperature (°C ⁻¹)
V_{nc}	Volume of test measure, compensated for deviation from reference temperature (L)
V_{mc}	Volume passing through the meter compensated for deviation from reference temperature (L)
\bar{E}	Mean value of error of indication (% or price)
n	Number of tests at the same condition
$P_c = V_i \times P_u$	
$E_v = (V_i - V_n) / V_n \times 100$	V_n may be replaced by V_{nc} , if appropriate.
$E_p = P_i \times P_c$	
$Q = (V_i \times 60) / t$	
$V_{nc} = V_n \times [1 + \beta (T - T_r)]$	
$\bar{E} = [E(1) + E(2) + \dots + E(n)] / n$	
Range	Maximum error – minimum error (% or price)

Note: If significant differences are recorded between the temperature of the liquid in the meter and the test measure, a correction on the liquid volume passing through the meter is computed as follows:

$$V_{mc} = V_{nc} \times [1 + \alpha (T_m - T)]$$

and in this case V_{nc} is to be replaced by V_{mc} in the whole text.

If β is not known, the following values can be used.

Material	β ($^{\circ}\text{C}^{-1}$) (uncertainty: $5 \times 10^{-6} \text{ }^{\circ}\text{C}^{-1}$)
Borosilica glass	10×10^{-6}
Glass	27×10^{-6}
Mild steel	33×10^{-6}
Stainless steel	51×10^{-6}
Copper, Brass	53×10^{-6}
Aluminium	69×10^{-6}

3.1 Determination of flowrate

The flowrate can be obtained under flying start/stop conditions by the following procedure:

- 1 Reset the volume indicator to zero. Insert the nozzle into a container of suitable capacity (see step 3 below), or back into the supply tank.
- 2 Start the pump. When the volume indication is at a whole number of litres, start the stop-watch. The volume indication at which the stop-watch was started should be noted.
- 3 After at least 30 seconds, stop the stop-watch when the volume indication is at a whole number of litres.
- 4 Calculate the flowrate Q from:

$$Q = V_i \times (60 / t)$$

where: V_i = the difference between the volume indication recorded at step 3 and the volume indication recorded at step 2, and t = the time elapsed in seconds, from the stop-watch in step 3.

3.2 Accuracy

Object of the test:

To verify that each measurement result at each flowrate meets the requirements concerning the maximum permissible errors.

Test procedure:

Regulate the flowrate accurately; use fixed positions of the nozzle valve or insert an adjustable full-flow valve between the nozzle and hose.

Before the endurance test, the dispenser is tested for accuracy at six flowrates from Q_{max} to Q_{min} (for blending dispensers at minimum and maximum grades plus at least one intermediate grade).

Three independent and identical tests shall be carried out at each flowrate.

Note: For blending dispensers, the maximum and minimum attainable flowrates may be different for each grade.

The six flowrates shall be calculated from:

$$Q = K^{n_F-1} \times Q_{\max}$$

where n_F is a sequence number of the flowrate test, and

$$K = \left[\frac{Q_{\min}}{Q_{\max}} \right]^{\frac{1}{N_F-1}}$$

where N_F is the number of flowrates.

When $Q_{\max}/Q_{\min} = 10$, this gives

$$\begin{aligned} Q(1) &= 1.00 \times Q_{\max} & (0.90 \times Q_{\max} \leq Q(1) \leq 1.00 \times Q_{\max}) \\ Q(2) &= 0.63 \times Q_{\max} & (0.56 \times Q_{\max} \leq Q(2) \leq 0.70 \times Q_{\max}) \\ Q(3) &= 0.40 \times Q_{\max} & (0.36 \times Q_{\max} \leq Q(3) \leq 0.44 \times Q_{\max}) \\ Q(4) &= 0.25 \times Q_{\max} & (0.22 \times Q_{\max} \leq Q(4) \leq 0.28 \times Q_{\max}) \\ Q(5) &= 0.16 \times Q_{\max} & (0.14 \times Q_{\max} \leq Q(5) \leq 0.18 \times Q_{\max}) \\ Q(6) &= 0.10 \times Q_{\max} = Q_{\min} & (0.10 \times Q_{\max} \leq Q(6) \leq 0.11 \times Q_{\max}) \end{aligned}$$

$$Q(2)/Q(1) = Q(3)/Q(2) = \dots = Q(6)/Q(5) = 0.63$$

For mechanical counters, the test shall be performed at not less than two unit prices which correspond to the maximum and minimum torques. This is generally near the maximum and minimum unit prices.

For electronic counters, the test shall be performed at the maximum unit price.

For both mechanical and electronic counters, one of the accuracy tests shall be performed at the maximum flowrate and maximum unit price stated in the application.

The test volume shall be determined such that the overall uncertainty does not exceed one-fifth of the maximum permissible error on pattern approval tests according to the provision in clause 6 of OIML R 117. The test measure shall not be smaller than the minimum measured quantity.

- 1 Set the maximum unit price P_u .
- 2 Adjust and determine the flowrate Q according to 3.1, steps 1 to 4.
- 3 Wet and drain the test measure.
- 4 Reset the indication of the dispenser.
- 5 Fill the test measure at the fixed flowrate, without stopping if possible.
- 6 Read P_u, V_i, P_i, V_n and T .
- 7 Calculate V_{nc}, P_c, E_v and E_p .
- 8 Drain the test measure.
- 9 Repeat steps 4 to 8 twice, and calculate the mean value of the errors E_v and the range of these errors.
- 10 Change the unit price, if applicable.
- 11 Repeat steps 2 to 10 at five other flowrates.
- 12 Repeat steps 1 to 11 at the above mentioned grades for blending dispenser only.
- 13 Draw a curve with \bar{E}_v as a function of Q for each grade (optional)

After the endurance test, the dispenser is tested for accuracy at three flowrates: $Q(1)$, $Q(4)$ and $Q(6)$. The unit price P_u shall be the same as that at the determination of the initial error curve.

3.3 Minimum measured quantity

Object of the test:

To determine the error of volume indication E_v when the dispenser delivers the minimum measured quantity.

Test equipment:

Test measure having a volume equal to the minimum measured quantity, as stated in the application.

Test procedure:

The dispenser is tested at Q_{\min} and, if possible, at the highest flowrate attainable with the test measure. Three independent and identical tests shall be executed at each flowrate.

- 1 Adjust and determine the flowrate Q according to 3.1, steps 1 to 4.
- 2 Wet and drain the test measure.
- 3 Reset the indication of the dispenser.
- 4 Fill the test measure at the fixed flowrate, without stopping if possible.
- 5 Read V_i , V_n and T .
- 6 Calculate V_{nc} and E_v .
- 7 Drain the test measure.
- 8 Repeat steps 4 to 7 twice.
- 9 Repeat steps 2 to 8 at the other flowrate if applicable.
- 10 Repeat steps 1 to 9 at the grades mentioned in 3.2 for blending dispenser only.

3.4 Flow interruption

Object of the test:

To determine the effect of sudden pressure variations on the accuracy of the volume and price indications.

Test procedure:

The interruption test shall be performed three times at the maximum flowrate. The test volume shall be at least the volume delivered in one minute at Q_{\max} . Using the nozzle valve, the liquid flow is started and stopped abruptly five times during the same measurement. These stops shall be made at various intervals.

The flowrate shall be determined according to 3.1, steps 1 to 4.

- 1 Set the maximum unit price P_u .
- 2 Adjust the flowrate to Q_{\max} .
- 3 Wet and drain the test measure.
- 4 Reset the indication of the dispenser.
- 5 Fill the test measure at Q_{\max} , with 5 stops.
- 6 Read P_u , V_i , P_i , V_n and T .
- 7 Calculate V_{nc} , P_c , E_v and E_p .
- 8 Drain the test measure.
- 9 Repeat steps 4 to 8 twice, and calculate the mean values \bar{E}_v and \bar{E}_p .
- 10 Repeat steps 1 to 9 at the grades mentioned in 3.2 for blending dispenser only.

3.5 Gas elimination device

Object of the test:

To determine the efficiency of the gas elimination device.

Test equipment:

Gas meter, valves, pressure gauge (where applicable) and a test measure with a capacity corresponding to at least the greater of:

- the volume delivered in one minute at the maximal flowrate,
- 1 000 times the scale interval, or
- the minimum measured quantity.

Test procedure:

Air is usually drawn into the dispenser through a special inlet, either upstream of the pump by suction, or downstream of the pump under pressure. In either case the air inlet should be fitted with a control valve, a stop valve and a non-return valve to prevent liquid from entering the inlet and draining out of the dispenser. Where the air is introduced under pressure, a pressure gauge shall be fitted as a means of measuring the air pressure in order to calculate the volume of air at atmospheric pressure. A schematic diagram of a typical piping arrangement is shown in Figure 1.

The air inlet can be open during the test. If a non-return valve is not fitted upstream of the pump, ensure that the open end of the air pipe, the control valve and the gas meter are all positioned above the highest liquid level in the dispenser.

A gas meter, complying with the requirements of International Recommendations OIML R 6 and R 31 or R 32, may be provided to measure the volume of the air (V_a).

Complete a test at Q_{max} without any air supply. Make at least six measurements with the control valve open in increasing amounts until the liquid flow from the pump stops. Draw an error curve as a function of supplied air.

The supplied air should be given as a relative value of the measured volume of liquid (V_a/V_n). The range of values of V_a/V_n is specified in Table 1. V_a is the volume of air isothermally converted to the atmospheric pressure.

Table 1

Viscosity of test liquid	With gas indicator	Without gas indicator
≤ 1 mPa.s	0 ~ 20 %	0 ~ ∞
> 1 mPa.s	0 ~ 10 %	

The test shall be performed at one grade (no blending).

- 1 Adjust initially the entry of air at 0 % at maximum liquid flowrate.
- 2 Wet and drain the test measure.
- 3 Run the dispenser for at least one minute to make sure the conditions are steady.
- 4 Do not switch off the dispenser. Read dispenser volume indication (V_{i1}) and gas meter indication (V_{a1}).
- 5 Fill the test measure at the maximum attainable flowrate.
- 6 Note any air bubbles in the gas indicator if fitted.
- 7 Read dispenser volume indication (V_{i2}) and gas meter indication (V_{a2}).
- 8 Calculate $V_i (= V_{i2} - V_{i1})$ and $V_a (= V_{a2} - V_{a1})$, and read V_n and T .
- 9 Calculate V_{nc} , E_v and V_a/V_n (or V_a/V_{nc} if appropriate).
- 10 Drain the test measure.
- 11 Repeat steps 2 to 9 at least five times in case of systems with gas indicator or until liquid flow stops after having increased the entry of air for each cycle by 4 % for liquids with viscosities not exceeding 1 mPa.s.

Notes

- (1) For fuel dispensers for diesel motor vehicles, this test shall be performed with diesel.
- (2) This test on the gas elimination device shall be performed at the maximum flowrate attainable by the liquid in the gas elimination device. Therefore adaptations of the abovementioned procedure shall be made according to the configuration of the dispenser.

3.6 Variation in the internal volume of hose

Object of the test:

To determine the increase in internal volume of a hose under pressure.

References:

International Standard ISO 6801 - 1983, *Rubber or plastics hoses - Determination of volumetric expansion.*

Test equipment:

A test installation, equipped with liquid supply, pressure source, a pressure gauge calibrated before test, a graduated cylindrical glass tube of suitable capacity, valves and piping, as illustrated in Figure 2.

Test procedure:

- 1 All valves should be closed before test.
- 2 Connect the hose in position on the test installation.
- 3 Open valves V_A , V_B and V_C , and fill the pressure source, the hose and the glass tube with liquid. Partially open valve V_D and allow the liquid to run from the tank through the glass tube until no air bubbles are seen in the glass tube. Then close all valves.
- 4 Open valve V_D , and adjust the liquid level to an appropriate position. Then close valve V_D , and read level X.

- 5 Open valve V_B . Adjust the pressure source until the reading of the pressure gauge is stable at the maximum operating pressure.
- 6 Close valve V_B .
- 7 Open valve V_C , and read level Y.
- 8 Calculate $Y - X$.
- 9 Close valve V_C .
- 10 Repeat steps 4 to 9 twice.
- 11 Calculate the mean value of $Y - X$.

3.7 Endurance test

Object of the test:

To determine the long term stability of the dispenser. (See subclause 6.1.5.3 of OIML R 117).

Test procedure:

When the dispenser is intended to measure different liquids, the test should be carried out with the liquid that provides the most severe conditions.

- 1 Check that the error curve is within the maximum permissible error (see 3.2).
- 2 Operate the dispenser for 100 hours (or 200 h in specific cases) at a flowrate between $0.8 \times Q_{\max}$ and Q_{\max} . For practical reasons, the volume may be divided in a number of deliveries.
- 3 Carry out the accuracy test after the endurance test at $Q(1)$, $Q(4)$ and $Q(6)$ according to 3.2.

Note: Additives may affect the long-term stability of the dispenser.

4 Additional testing procedures for electronic dispensers

For fuel dispensers equipped with electronic devices, the following tests shall be performed in addition to the tests specified in clause 3. Test procedures are given in condensed form, adapted from the mentioned IEC publications. Before conducting tests, consult the applicable IEC Publication.

Where size and configuration permit, tests shall be carried out on the complete dispenser. Otherwise, (except in the case of the electrostatic discharge and electromagnetic susceptibility tests) the tests may be carried out separately on the following electronic devices:

- measuring transducer,
- calculator,
- indicating device,
- power supply device, and
- correction device, if appropriate.

Insofar as electrostatic discharges and electromagnetic susceptibility tests are concerned, the approving authority may decide to perform the tests either on the complete dispenser or on the calculator, on the basis of their configuration; it may also decide that a pattern approval covering a given pattern of dispenser with a given housing will cover any other housing of the same pattern.

The equipment under test (if other than the complete dispenser) shall be included in a simulation set-up representative of the normal operation of the dispenser. For example, the movement of liquid may be simulated by rotating the shaft of the pulse generator.

During these tests the equipment under test (EUT) shall be operational (i.e. the power shall be switched on) except for the damp heat cyclic (condensing) test (4.3).

4.1 Dry heat (non condensing)

(Influence factor)

Object of the test:

To verify that the errors of volume and price indications do not exceed the maximum permissible errors under the effect of high temperature. All other functions shall operate correctly.

References:

IEC Publication 68-2-2, fourth edition, 1974, Basic environmental testing procedures, Part 2: Tests, Test Bd: Dry heat, for heat dissipating equipment under test EUT with gradual change of temperature.

Background information concerning dry heat tests is given in IEC Publication 68-3-1, first edition, 1974 and first supplement 68-3-1A, 1978, Part 3: Background information, section one; Cold and dry heat tests. General background information on basic environmental testing procedures is given in IEC Publication 68-1, sixth edition, 1988.

Test equipment:

Testing chamber capable of maintaining the specified temperatures within ± 2 °C.

Test procedure:

- 1 Maintain the EUT at 20 °C for at least two hours.
- 2 Set the unit price at an optional value between the minimum unit price and the maximum unit price, and select blending if applicable.
- 3 Adjust the flowrate or the simulated flowrate at an appropriate value between $0.5 \times Q_{\max}$ et Q_{\max} .
- 4 Reset the indications of the dispenser.
- 5 Operate the pump or the pulse generator at a rate equivalent to the volume flow for one minute at the maximum flowrate. (In general, 50 litres may be the appropriate value for the volume flow for normal dispensers).
- 6 Read P_u , V_p , P_i and V_n . (Read T only in the case of test by liquid flow).
- 7 Calculate P_c , V_{nc} (only in the case of test by liquid flow), E_v and E_p .
- 8 Change the temperature of the EUT to 55 °C at a rate not exceeding 1 °C/min. Maintain this temperature for at least two hours after it has reached stability. The humidity shall not exceed 20 g/m³ or 19 % RH.
- 9 Repeat steps 4 to 7.
- 10 Return the temperature of the EUT to 20 °C at a rate not exceeding 1 °C/min. Maintain this temperature for at least 2 hours after it has reached stability.
- 11 Repeat steps 4 to 7.

4.2 Cold

(Influence factor)

Object of the test:

To verify that the errors of volume and price indications do not exceed the maximum permissible errors under the effect of low temperature. All other functions shall operate correctly.

References:

IEC Publication 68-2-2, fourth edition, 1974, Basic environmental testing procedures, Part 2: Tests, Test Ad: Cold, for heat dissipating EUT with gradual change temperature.

Background information concerning cold tests is given in IEC Publication 68-3-1, first edition, 1974 and first supplement 68-3-1A, 1978, Part 3: Background information, section one: Cold and dry heat tests. General background information on basic environmental testing procedures is given in IEC Publication 68-1, sixth edition, 1988.

Test equipment:

Testing chamber capable of maintaining the specified temperatures within ± 2 °C.

Test procedure:

- 1 Maintain the EUT at 20 °C for at least two hours.
- 2 Set the unit price at an optional value between the minimum unit price and the maximum unit price, and select blending if applicable.
- 3 Adjust the flowrate or the simulated flowrate at an appropriate value between $0.5 \times Q_{\max}$ and Q_{\max} .
- 4 Reset the indications of the dispenser.
- 5 Operate the pump or the pulse generator at a rate equivalent to the volume flow for one minute at the maximum flowrate.
- 6 Read P_u , V_i , P_i and V_n . (Read T only in the case of test by liquid flow).
- 7 Calculate P_c , V_{nc} (only in the case of test by liquid flow), E_v and E_p .
- 8 Change the temperature of the EUT to -25 °C at a rate not exceeding 1 °C/min. Maintain this temperature for at least two hours after it has reached stability.
- 9 Repeat steps 4 to 7.
- 10 Return the temperature of the EUT to 20 °C at a rate not exceeding 1 °C/min. Maintain this temperature for at least two hours after it has reached stability.
- 11 Repeat steps 4 to 7.

4.3 Damp heat, cyclic (condensing)

(Influence factor)

Object of the test:

To verify that the errors of volume and price indications do not exceed the maximum permissible errors after exposing the EUT to the effect of high humidity, combined with cyclic temperature changes. All other functions shall operate correctly.

References:

IEC Publication 68-2-30, second edition, 1980, Basic environmental testing procedures, Part 2: Tests, test Db: Damp heat, cyclic (12 h + 12 h cycle), test variant 1.

Background information concerning damp heat tests is given in IEC Publication 68-2-28, second edition, 1980: Guidance for damp heat tests.

Test equipment:

Testing chamber capable of maintaining the specified temperature within $\pm 2\text{ }^{\circ}\text{C}$ and the relative humidity within $\pm 3\text{ }%$.

Test procedure:

- 1 Maintain the EUT at $20\text{ }^{\circ}\text{C}$ and the relative humidity of $50\text{ }%$ for at least two hours.
- 2 Set the unit price at an optional value between the minimum unit price and the maximum unit price, and select blending if applicable.
- 3 Adjust the flowrate or the simulated flowrate at an appropriate value between $0.5 \times Q_{\max}$ and Q_{\max} .
- 4 Reset the indications of the dispenser.
- 5 Operate the pump or the pulse generator at a rate equivalent to the volume flow for one minute at the maximum flowrate.
- 6 Read P_u , V_i , P_i and V_n . (Read T only in the case of test by liquid flow).
- 7 Calculate P_c , V_{nc} (only in the case of test by liquid flow), E_v and E_p .
- 8 After switching off the power, change the temperature of the EUT from $20\text{ }^{\circ}\text{C}$ to $25\text{ }^{\circ}\text{C}$ and the relative humidity above $95\text{ }%$.
- 9 Change the temperature of the EUT from $25\text{ }^{\circ}\text{C}$ to $55\text{ }^{\circ}\text{C}$ during three hours maintaining the relative humidity above $95\text{ }%$ during the temperature change and lower temperature phases. Condensation should occur on the EUT during the temperature rise.
- 10 Maintain the temperature of $55\text{ }^{\circ}\text{C}$ and the relative humidity of $95\text{ }%$ until 12 hours from the start of the temperature rise.
- 11 Change the temperature of the EUT from $55\text{ }^{\circ}\text{C}$ to $25\text{ }^{\circ}\text{C}$ within three to six hours maintaining the relative humidity above $95\text{ }%$ during the temperature change and lower temperature phases. In the first half fall, the temperature should be lowered from $55\text{ }^{\circ}\text{C}$ to $40\text{ }^{\circ}\text{C}$ in one and a half hour.
- 12 Maintain the temperature of $25\text{ }^{\circ}\text{C}$ and the relative humidity above $95\text{ }%$ until 24 hours from the start of the temperature rise.
- 13 Repeat steps 9 to 12.
- 14 Return the temperature of the EUT to $20\text{ }^{\circ}\text{C}$ and the relative humidity to $50\text{ }%$, and switch on the power. Maintain this temperature and relative humidity for at least two hours after it has reached stability.
- 15 Repeat steps 2 to 7.

4.4 Power voltage variations

(Influence factor)

Object of the test:

To verify that the errors of volume and price indications do not exceed the maximum permissible errors under the effect of varying mains power supply. All other functions shall operate correctly.

References:

No reference to an international standard can be given at the present time.

Test equipment:

Voltage regulator

Test procedure:

- 1 Maintain the EUT at the reference conditions.
- 2 Set the unit price at an optional value between the minimum unit price and the maximum unit price, and select blending if applicable.
- 3 Adjust the flowrate or the simulated flowrate at an appropriate value between $0.5 \times Q_{\max}$ and Q_{\max} .
- 4 Reset the indications of the dispenser.
- 5 Operate the pump or the pulse generator at a rate equivalent to the volume flow for one minute at the maximum flowrate.
- 6 Read P_u , V_i , P_i and V_n . (Read T only in the case of test by liquid flow).
- 7 Calculate P_c , V_{nc} (only in the case of test by liquid flow), E_v and E_p .
- 8 Change the mains voltage to 110 % of the nominal value.
- 9 Repeat steps 4 to 7.
- 10 Change the mains voltage to 85 % of the nominal value.
- 11 Repeat steps 4 to 7.

4.5 Short-time power reductions

(Disturbance)

Object of the test:

To verify, under the effect of short-time interruptions and reductions in mains voltage, that either significant faults do not occur or significant faults are detected and acted upon by means of a checking facility.

References:

No reference to international standard can be given at the present time.

Test equipment:

Test generator suitable to reduce the amplitude of one or more half cycles (at zero crossings) of the AC mains voltage.

Test procedure:

- 1 Maintain the EUT at the reference conditions.
- 2 Adjust the test generator to the specified conditions and connect it to the EUT.
- 3 Set the unit price at an optional value between the minimum unit price and the maximum unit price, and select blending if applicable.
- 4 Adjust the flowrate or the simulated flowrate at an appropriate value between $0.5 \times Q_{\max}$ and Q_{\max} .
- 5 Reset the indications of the dispenser.
- 6 Operate the pump or the pulse generator at a rate equivalent to the volume flow for about two minutes at the maximum flowrate.
- 7 Read P_u , V_i , P_i and V_n . (Read T only in the case of test by liquid flow).
- 8 Calculate P_c , V_{nc} (only in the case of test by liquid flow), E_v and E_p .
- 9 Reset the indications of the dispenser.

- 10 Start the pump or the pulse generator.
- 11 Reduce the mains voltage to 100 % for half a cycle and repeat nine times with an interval of at least 10 seconds.
- 12 Stop the pump or the pulse generator at the same volume flow or number of pulses as in step 6.
- 13 Repeat steps 7 and 8.
- 14 Repeat steps 9 and 10.
- 15 Reduce the mains voltage by 50 % for one cycle and repeat nine times with an interval of at least ten seconds.
- 16 Stop the pump or the pulse generator at the same volume flow or number of pulses as in step 6.
- 17 Repeat steps 7 and 8.

4.6 Electrical bursts

(Disturbance)

Object of the test:

To verify, when electrical bursts are superimposed on the mains voltage, that either significant faults do not occur or significant faults are detected and acted upon by means of a checking facility.

References:

IEC Publication 801-4, first edition, 1988, Electromagnetic compatibility for industrial-process measurement and control equipment, Part 4: Electrical fast transient/burst requirements.

Test equipment:

Test generator having an output impedance of 50 Ω , and capable of superimposing electrical bursts, of which each spike has a peak value of 1 kV, a rise time of 5 ns, a burst length of 15 ms and a burst period (repetition time interval) of 300 ms, on the AC mains voltage.

Test procedure:

- 1 Maintain the EUT at the reference conditions.
- 2 Adjust the test generator to the specified conditions and connect to the EUT.
- 3 Set the unit price at an optional value between the minimum unit price and the maximum unit price, and select blending if applicable.
- 4 Adjust the flowrate or the simulated flowrate at an appropriate value between $0.5 \times Q_{\max}$ and Q_{\max} .
- 5 Reset the indications of the dispenser.
- 6 Operate the pump or the pulse generator at a rate equivalent to the volume flow for one minute at the maximum flowrate.
- 7 Read P_w , V_i , P_i and V_n . (Read T only in the case of test by liquid flow).
- 8 Calculate P_c , V_{nc} (only in the case of test by liquid flow), E_v and E_p .
- 9 Set the test generator in a non-symmetrical condition between the reference ground and one line of the AC mains power supply.
- 10 Reset the indications of the dispenser.
- 11 Start the pump or the pulse generator.
- 12 Apply ten positive, randomly-phased bursts, each of which has a length of 15 ms and a repetition time interval of 300 ms.

- 13 Stop the pump or the pulse generator at the same volume flow or number of pulses as in step 6.
- 14 Repeat steps 7 and 8.
- 15 Repeat steps 10 and 11.
- 16 Apply ten negative, randomly-phased bursts in the same way as in step 12.
- 17 Stop the pump or the pulse generator at the same volume flow or number of pulses as in step 6.
- 18 Repeat steps 7 and 8.
- 19 Set the test generator in a non-symmetrical condition between the reference ground and the other line of the AC mains power supply.
- 20 Repeat steps 10 to 18.

4.7 Electrostatic discharges (Disturbance)

Object of the test:

To verify, under the effect of electrostatic discharges, that either significant faults do not occur or significant faults are detected and acted upon by means of a checking facility.

References:

IEC Publication 801-2, second edition, 1991, Electromagnetic compatibility for industrial-process measurement and control equipment, Part 2: Electrostatic discharge requirements.

Test equipment:

Test equipment having a capacitor of 150 pF, which is able to be charged up to 8 kV DC voltage and then discharged through the EUT, or vertical or horizontal coupling plate (VCP or HCP) by connecting one terminal to the ground (earth reference plane) and the other via 330 Ω resistance to the surfaces of the EUT, or VCP or HCP.

Test procedure:

Both direct and indirect discharges shall be applied including the paint penetration method.

When contact discharges (test voltage: 6 kV) are not possible, air discharges (test voltage: 8 kV) shall be applied.

- 1 Maintain the EUT at the reference conditions.
- 2 Adjust the test equipment to the specified conditions.
- 3 Set the unit price at an optional value between the minimum unit price and the maximum unit price, and select blending if applicable.
- 4 Adjust the flowrate or the simulated flowrate at an appropriate value between $0.5 \times Q_{\max}$ and Q_{\max} .
- 5 Reset the indications of the dispenser.
- 6 Operate the pump or the pulse generator at a rate equivalent to the volume flow for about two minutes at the maximum flowrate.
- 7 Read P_u , V_i , P_i and V_n . (Read T only in the case of test by liquid flow).
- 8 Calculate P_c , V_{nc} (only in the case of test by liquid flow), E_v and E_p .
- 9 Reset the indications of the dispenser.

- 10 Start the pump or the pulse generator.
- 11 Apply at least ten discharges, at intervals of at least ten seconds, to a point on a surface which is normally accessible to the operator.
- 12 Stop the pump or the pulse generator at the same volume flow or number of pulses as in step 6.
- 13 Repeat steps 7 and 8.
- 14 Repeat steps 9 to 13. However, in step 11 apply the discharges to other points and surfaces which are normally accessible to the operator. The number of times this step is repeated will depend upon the type and configuration of the EUT, but as many surfaces as practical shall be tested.
- 15 Repeat steps 9 to 13. However, in step 11 apply the discharge to the VCP or HCP.

4.8 Electromagnetic susceptibility (Disturbance)

Object of the test:

To verify, under the effect of electromagnetic fields, that either significant faults do not occur or significant faults are detected and acted upon by means of a checking facility.

References:

IEC Publication 801-3, second edition, 1991, Electromagnetic compatibility for electrical and electronic equipment, Part 3: Immunity to radiated, radio frequency, electromagnetic fields.

Test equipment:

Signal generator(s) capable of generating 80 % AM 1 kHz sine wave with the frequency range from 26 to 1 000 MHz, power amplifier(s), antenna system capable of satisfying frequency requirements, a transverse electromagnetic (TEM) cell, field strength monitoring system, and a shielded room.

Test procedure:

With the antenna method, the test is normally performed with the EUT rotating on an insulated table. The polarization of the field generated by the antenna necessitates testing each position twice, once with the antenna positioned vertically and again with the antenna positioned horizontally.

With the TEM cell method, the EUT is normally tested in three mutually perpendicular axes. However, the test can be performed with the EUT in the most sensitive orientation, if applicable.

- 1 Maintain the EUT at the reference conditions.
- 2 Set the unit price at an optional value between the minimum unit price and the maximum unit price, and select blending if applicable.
- 3 Adjust the flowrate or simulated flowrate at an appropriate value between $0.5 \times Q_{\max}$ and Q_{\max} .
- 4 Reset the indications of the dispenser.
- 5 Operate the pump or the pulse generator at a rate equivalent to the volume flow for the estimated duration long enough for sweeping the frequency in step 12 (or in step 19).
- 6 Read P_u , V_i , P_i and V_n . (Read T only in the case of test by liquid flow).

- 7 Calculate P_c , V_{nc} (only in the case of test by liquid flow), E_v and E_p .
- 8 Keep the shielded room (or the TEM cell) at the reference conditions, and adjust the field strength to 3 V/m. When the shielded room (antenna method) is used, set the antenna at the height of 1 m and adjust the field strength to 3 V/m at the horizontal distance of 1 m from the antenna.
- 9 Set the EUT at the place where the field strength was adjusted to 3 V/m in the shielded room (or the TEM cell).
- 10 Reset the indications of the dispenser.
- 11 Start the pump or the pulse generator.
- 12 Sweep the frequency from 26 MHz to 500 MHz. The sweep velocity shall not exceed 0.005 octave/s (1.5×10^{-3} decades/s).
- 13 Stop the pump or the pulse generator at the same volume flow or number of pulses as in step 5.
- 14 Repeat steps 6 and 7.
- 15 Remove the EUT from the shielded room (or TEM cell).
- 16 Adjust the field strength to 1 V/m. When the shielded room (antenna method) is used, set the antenna at a height of 1 m and adjust the field strength to 1 V/m at the horizontal distance of 1 m from the antenna.
- 17 Set the EUT at the place where the field strength was adjusted to 1 V/m in the shielded room (or TEM cell).
- 18 Repeat steps 10 and 11.
- 19 Sweep the frequency from 500 MHz to 1 000 MHz. The sweep velocity shall not exceed 0.005 octave/s (1.5×10^{-3} decades/s).
- 20 Repeat steps 13 and 14.

Notes

- (1) When this test is performed with liquid flow in the actual operating conditions, the above detailed procedure must be modified accordingly.
- (2) The above procedure may be modified according to the configuration of the EUT and of the test equipment.

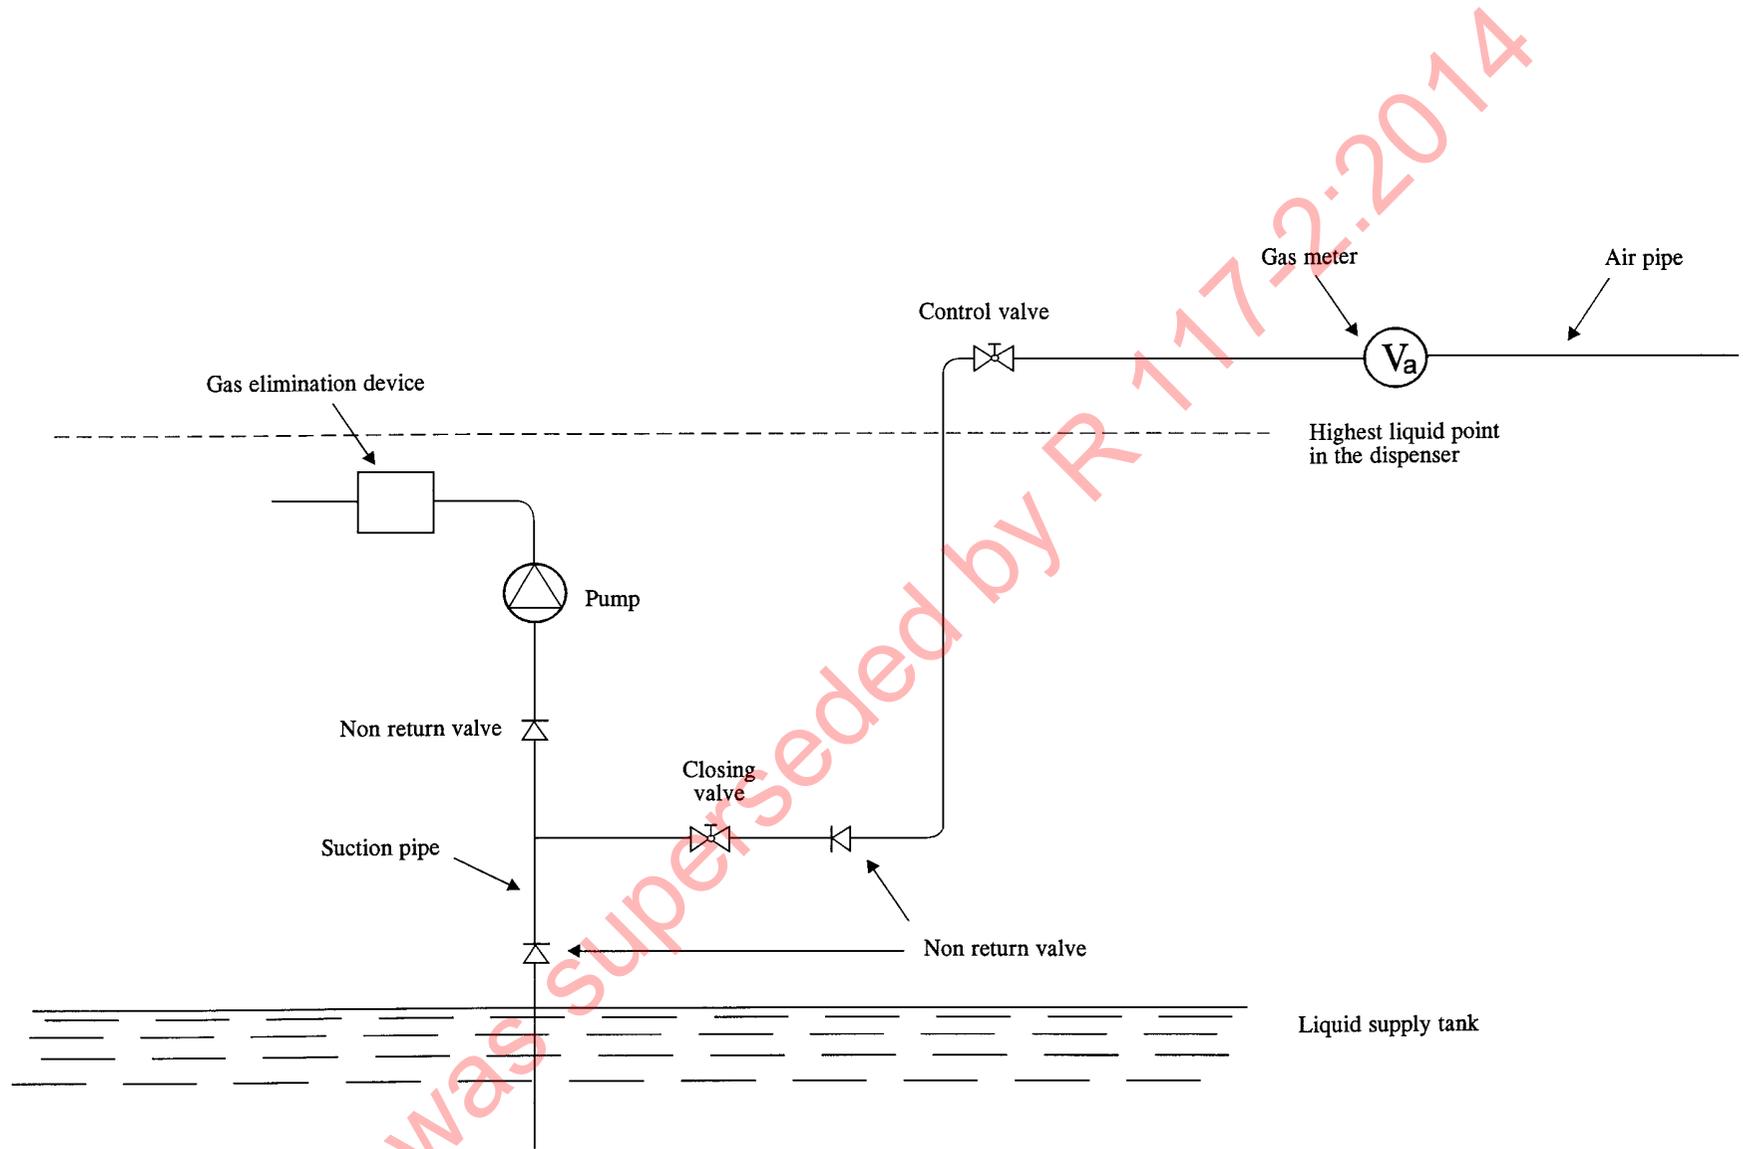


Figure 1 - Installation for gas elimination device test

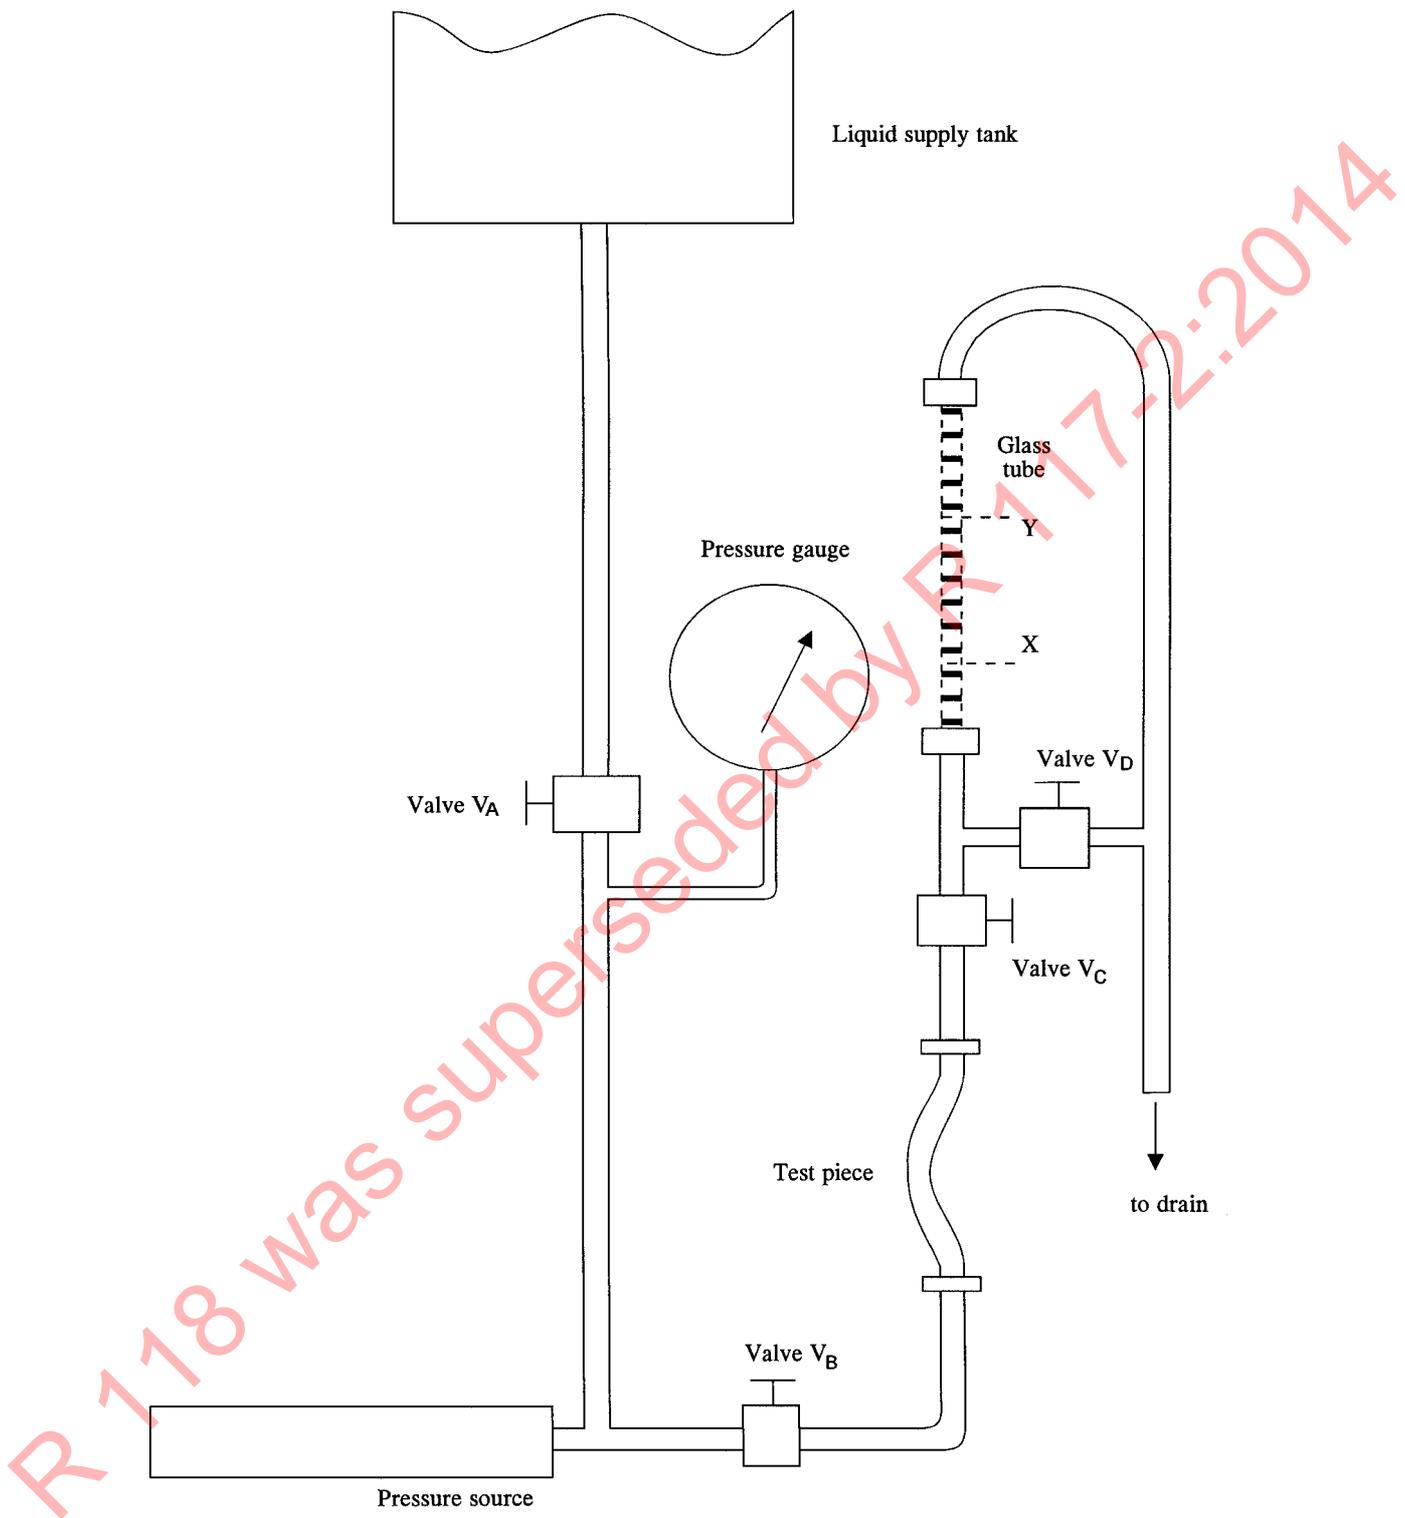


Figure 2 - Test apparatus for variation in the internal volume of hose

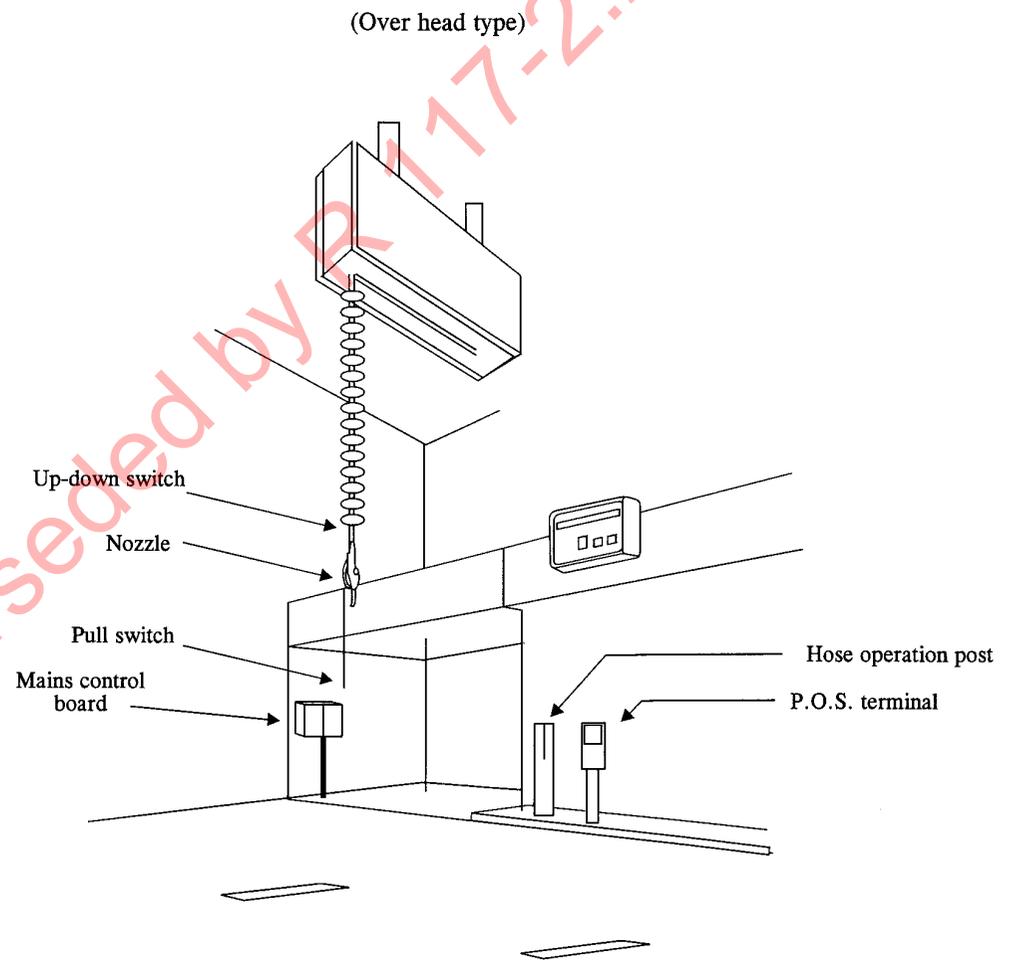
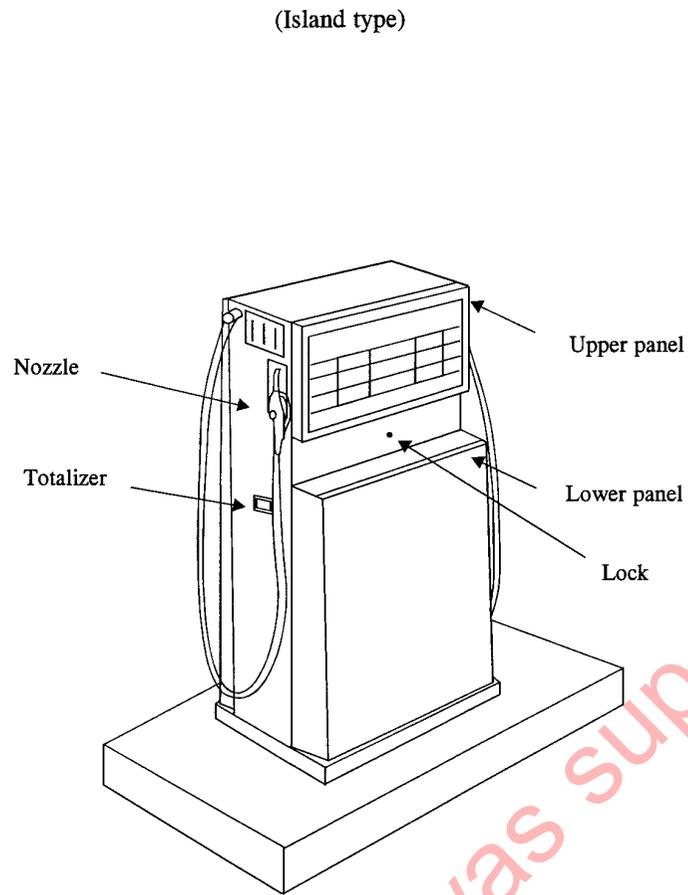


Figure 3 - Schematic installation of fuel dispensers

ANNEX A

TEST REPORT FORMAT

Note: This Annex is informative with regard to the implementation of OIML R 117 and of the present Recommendation in national regulations; however, use of the test report format is mandatory for application of OIML R 117 and of the present Recommendation within the OIML Certificate System.

The test report given in this Annex aims at presenting, in a standardized format, the results of the various tests described in this Recommendation, and to which a pattern of a fuel dispenser for motor vehicles shall be submitted with a view to its approval according to the requirements of the International Recommendation OIML R 117 *Measuring systems for liquids other than water*.

The symbols used in this Annex are:

- + = Passed
- = Failed
- mpe = Maximum permissible error
- MMQ = Minimum measured quantity
- MSVD = Minimum specified volume deviation
- MSPD = Minimum specified price deviation

For each test, the “check list shall be completed according to this example:

+	-	
×		if the instrument has passed the test
	×	if the instrument has failed
/	/	if the test is not applicable

GENERAL INFORMATION CONCERNING THE PATTERN

Application No.: (new/modification)

Manufacturer:

Applicant:

Representative:

Measuring system

Pattern designation:

Maximum flowrate: Minimum flowrate:

Minimum measured quantity:

Maximum unit price (number of digits):

Maximum price to pay (number of digits):

Temperature range:

Liquids (or viscosity range):

Mains power:

Voltage: Frequency: Consumption:

Type of display: mechanical/electromechanical/electronic

Meter

Manufacturer:

Pattern designation: Pattern approval mark:

Maximum flowrate: Minimum flowrate:

Minimum measured quantity:

Gas elimination device

Manufacturer:

Pattern designation: Pattern approval mark:

Volume:

Maximum flowrate: Minimum flowrate:

Maximum pressure: Minimum pressure:

Measuring transducer

Manufacturer:

Pattern designation: Pattern approval mark:

Number of pulses per revolution:

General information on other devices, e.g. calculator, indicating device, printing device, delivery unit (hose, nozzle), etc., which have been subject to testing, and a description of the configuration of the complete dispenser shall be given.

CHECK LIST

Note: Item numbering refers to International Recommendation OIML R 117 *Measuring systems for liquids other than water*.

§ (R 117)	Requirement	+	-	Remarks
GENERAL PROVISIONS				
2.19.1	MARKINGS Markings applied legibly and indelibly on the dial of the indicating device or on a special data plate: <ul style="list-style-type: none"> • Pattern approval sign • Manufacturer's identification mark or trade mark designation • Serial number • Year of manufacture • Minimum measured quantity (MMQ) • Maximum flowrate (Q_{\max}) • Minimum flowrate (Q_{\min}) • Maximum pressure • Minimum pressure • Liquids • Temperature range 			
2.9.1	INDICATIONS Unit of volume: litre (l or L)			
2.9.5	Difference between volume indications of more than one indicating device ≤ 1 scale interval of indicating device with the greatest scale interval			
2.16.1	BRANCHES AND BY-PASSES Branches downstream of meter: diversion to any receiving receptacle(s) other than that intended is impossible			
2.20.1	SEALING DEVICES AND STAMPING PLATE Seals easily accessible and preventing access to components which allow alteration of the measurement result without damaging the seals including the stamping plate			
REQUIREMENTS FOR ANCILLARY DEVICES OF A MEASURING SYSTEM				
3.1.4	ADJUSTMENT DEVICE Difference between consecutive values of the ratio ≤ 0.001 Adjustment by means of a by-pass of the meter impossible			

§ (R 117)	Requirement	+	-	Remarks
	VOLUME INDICATING DEVICE			
3.2.1.1	Reading precise, easy and unambiguous by simple juxtaposition Decimal sign clear			
3.2.1.2	Scale interval: 1×10^n , 2×10^n or 5×10^n			
3.2.1.4	Continuous indicating device: MSVD \geq volume corresponding to 2 mm on the scale, and $\geq 1/5$ of scale interval Discontinuous indicating device: MSVD ≥ 2 scale intervals			
3.2.2.1	Element with graduation entirely visible (except element corresponding to the maximum range of the indicator): one revolution corresponds to 10^n authorized units of volume			
3.2.2.2	Element with graduation entirely visible: one revolution of the element corresponds to scale interval of the following element			
3.2.2.3	Element with only part of graduation visible through a window (except first element): discontinuous movement			
3.2.2.4	Advance by one figure of following element when preceding element passes from 9 to 0			
3.2.2.5	Dimension of the window for the first element $\geq 1.5 \times$ (distance between two graduated scale marks)			
3.2.2.6	Width of scale mark $\leq 1/4$ of scale spacing Apparent scale spacing ≥ 2 mm			
3.2.3	Electronic indicating device: continuous display of volume during the period of measurement			
3.2.4.2	Zero setting device not permitting any alteration of the result			
3.2.4.3	No indication of any result during zeroing			
3.2.4.4	Continuous indicating device: residual indication after zeroing $\leq 1/2$ of MSVD			
3.2.4.5	Discontinuous indicating device: indicate zero without any ambiguity			
	PRICE INDICATING DEVICE			
3.3.2	Unit price adjustable and indicated before measurement by a displaying device; valid for the whole transaction Elapsed time between changing unit price and before next measurement starts: at least five seconds			

§ (R 117)	Requirement	+	-	Remarks
3.3.3 (3.2.1.1) (3.2.2.4) (3.2.4.2) (3.2.4.3)	(mutatis mutandis) Reading precise, easy and unambiguous Advance by figure of following element when preceding element passes from 9 to 0 Zero setting device not permitting any alteration of the result No indication of any result during zeroing			
3.3.4	Monetary unit or its symbol in the immediate vicinity of the indicating device			
3.3.5	Zero setting devices of price indication and volume indication: zeroing of either of them automatically involves zeroing the other			
3.3.6	Continuous indicating device: MSPD \geq price corresponding to 2 mm on the scale, and \geq price corresponding to 1/5 of scale interval Discontinuous indicating device: MSPD \geq price corresponding to 2 scale intervals			
3.3.8	Continuous indicating device: residual indication after zeroing \leq 1/2 of MSPD			
3.3.9	Discontinuous indicating device: indicate zero without any ambiguity			
	PRINTING DEVICE			
3.4.1	Printed volume scale interval: 1×10^n , 2×10^n or 5×10^n , and \leq MSVD, and \geq smallest scale interval of indicating device			
3.4.2	Unit of volume: litre (l or L) Figures, unit or symbol, (and decimal sign) of volume printed on ticket			
3.4.3	If connected to more than one measuring system: print identification			
3.4.4	If repetition of printing: copies are marked clearly			
3.4.5	If volume determination by difference between two printed values: withdrawal of ticket during measurement impossible			
3.4.6	Zeroing device of printer and volume indicator: zeroing of one of them involves zeroing the other			
3.4.7	Figures, monetary unit or symbol, (and decimal sign) of price printed on ticket			

§ (R 117)	Requirement	+	-	Remarks
3.4.8	Printed price scale interval: 1×10^n , 2×10^n or 5×10^n monetary unit, and \leq MSPD			
	PRE-SETTING DEVICE			
3.6.2	If several independent controls: scale interval corresponding to one control equals range of control of the next lower order			
3.6.4	Figures of pre-setting display clearly distinguishable from those of volume indicator			
3.6.5	Indication of the selected quantity during delivery remains unaltered or returns progressively to zero			
3.6.6	Difference between pre-set volume and indicated volume \leq MSVD			
3.6.7	Unit of pre-set volume same as that of volume indicator Marking of unit of volume or its symbol on pre-setting mechanism			
3.6.8	Scale interval of pre-setting device \geq scale interval of volume indicator			
3.6.10	(mutatis mutandis for price pre-setting devices)			
(3.6.2)	If several independent controls: scale interval corresponding to one control equals range of control of the next lower order			
(3.6.4)	Figures of pre-setting display clearly distinguishable from those of price indicator			
(3.6.5)	Indication of the selected quantity during delivery remains unaltered or returns progressively to zero			
(3.6.6)	Difference between pre-set price and indicated price \leq MSPD			
(3.6.7)	Unit of pre-set price same as that of price indicator Marking of monetary unit or its symbol on pre-setting mechanism			
(3.6.8)	Scale interval of pre-setting device \geq scale interval of price			

§ (R 117)	Requirement	+	-	Remarks
SPECIFIC REQUIREMENTS FOR MEASURING SYSTEMS EQUIPPED WITH ELECTRONIC DEVICES				
4.3.2.1	<p>CHECKING FACILITIES FOR MEASUREMENT TRANSDUCER</p> <p>When each pulse represents elementary volume, at least security level B defined by ISO 6551</p> <p>Checking facilities of type P</p> <p>Checking interval not exceeding the duration of measurement of amount of liquid equal to MSVD</p> <p>Possibility of testing the operation of checking facilities during pattern approval and verification</p>			
4.3.3.1	<p>CHECKING FACILITIES FOR CALCULATION</p> <p>Checking facilities for operation of type P or I</p> <p>Checking interval for type I at each delivery</p>			
4.3.3.2	<p>Checking facilities for validity of calculation of type P</p> <p>Existence of a means for controlling continuity</p>			
4.3.4.1	<p>CHECKING FACILITIES FOR INDICATING DEVICE</p> <p>Checking facilities of type P or I if indication can be reconstituted</p>			
4.3.4.2	<p>Tests "all displaying" - "all blanking" - "all zeros" test with duration of each sequence ≥ 0.75 s</p>			
4.3.4.3	<p>Possibility of testing the operation of checking facilities during verification</p>			
4.3.5	<p>CHECKING FACILITIES FOR PRINTING DEVICE</p> <p>Checking facilities of type I or P</p> <p>Checking includes presence of paper and of electronic control circuits</p> <p>Possibility of testing the operation of checking facilities during pattern approval and verification</p> <p>Where action is a warning: given on or by the printing device</p>			

§ (R 117)	Requirement	+	-	Remarks
OTHER SPECIFIC REQUIREMENTS FOR FUEL DISPENSERS				
5.1.1	Ratio between maximum flowrate and minimum flowrate: at least ten			
5.1.2	If integral pump: gas elimination device placed immediately upstream of the meter inlet			
5.1.3	If no integral pump: check that the installation schemes provide for necessary securities			
5.1.4	Device for resetting the volume indicator to zero present Height of figures of volume indicator with zero setting device ≥ 10 mm If price indicator, presence of zero setting device			
5.1.5	Next delivery inhibited until nozzle(s) replaced and indicator reset to zero			
5.1.6	When maximum flowrate (Q_{\max}) ≤ 3.6 m ³ /h, MMQ ≤ 5 L			
5.1.8	Fuel dispenser interruptible			
5.1.9	Minimum duration of operation of display after power failure ≥ 15 min continuously and automatically, or ≥ 5 min in one or several periods controlled manually during 1 h Delivery interrupted by power failure: impossible to continue delivery if power failure has lasted more than 15 s			
5.1.10	Delay time between measurement value and indicated values ≤ 500 ms			
5.1.12	Hidden volume at the beginning of the delivery $\leq 2 \times$ MSVD Hidden price at the beginning of the delivery $\leq 2 \times$ MSPD			

CONCLUSION OF TESTS

Application No.:

Date:

Certificate of Conformity No.:

Date:

N°	Test description	+	-	Remarks
1	Accuracy			
2	Minimum measured quantity			
3	Flow interruption			
4	Gas elimination device			
5	Variation in the internal volume of hose			
6	Endurance test			
7	Dry heat (non-condensing)			
8	Cold			
9	Damp heat, cyclic (condensing)			
10	Power voltage variations			
11	Short-time power reductions			
12	Electrical burst			
13	Electrostatic discharges			
14	Electromagnetic susceptibility			

Notes:

+	-
×	/
/	×
/	/

if the instrument has passed the test

if the instrument has failed

if the test is not applicable

Remarks:

Observer: _____

TEST REPORT

Symbols, units and equations:

P_u	Unit price (price/L)
t	Time (s)
Q	Flowrate of liquid (L/min)
V_i	Volume indication of dispenser (L)
P_i	Price indication (or printed if not fitted with a price indicator) of dispenser (price)
P_c	Calculated price (price)
V_n	Volume indication of test measure or computed volume from simulated pulses (L)
T	Temperature of liquid in the test measure (°C)
T_r	Reference temperature of test measure (°C)
T_m	Temperature of liquid passing through the meter (°C)
E_v	Error of volume indication (%)
E_p	Error of price indication (price)
Q_a	Flowrate of air (L/min)
V_a	Volume of air (L)
α	Cubic expansion coefficient of test liquid due to temperature (°C ⁻¹)
β	Cubic expansion coefficient of test measure due to temperature (°C ⁻¹)
V_{nc}	Volume of test measure, compensated for deviation from reference temperature (L)
V_{mc}	Volume passing through the meter compensated for deviation from reference temperature (L)
\bar{E}	Mean value of error of indication (% or price)
n	Number of tests at the same condition
P_c	$= V_i \times P_u$
E_v	$= (V_i - V_n) / V_n \times 100$ V_n may be replaced by V_{nc} , if appropriate
E_p	$= P_i \times P_c$
Q	$= (V_i \times 60) / t$
V_{nc}	$= V_n \times [1 + \beta (T - T_r)]$
\bar{E}	$= [E(1) + E(2) + \dots + E(n)] / n$
Range	= Maximum error – minimum error (% or price)

Note: If significant differences are recorded between the temperature of the liquid in the meter and the test measure, a correction on the liquid volume passing through the meter is computed as follows:

$$V_{mc} = V_{nc} \times [1 + \alpha (T_m - T)]$$

and in this case V_{nc} is to be replaced by V_{mc} in the whole text.

If β is not known, the following values can be used.

Material	β (°C ⁻¹) (uncertainty: 5×10^{-6} °C ⁻¹)
Borosilica glass	10×10^{-6}
Glass	27×10^{-6}
Mild steel	33×10^{-6}
Stainless steel	51×10^{-6}
Copper, Brass	53×10^{-6}
Aluminium	69×10^{-6}

1 Accuracy

Q() L/min	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	mpe %	E_p Price	MSPD Price
\bar{E}_v	%		Range	%		\bar{E}_p					

Q() L/min	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	mpe %	E_p Price	MSPD Price
\bar{E}_v	%		Range	%		\bar{E}_p					

Q() L/min	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	mpe %	E_p Price	MSPD Price
\bar{E}_v	%		Range	%		\bar{E}_p					

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Test measures used: _____

β : _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s

Grade: _____

Ambient conditions

Temperature: _____ °C

Humidity: _____ % RH

Pressure: _____ hPa

Remarks:

2 Minimum measured quantity

Q L/min	V_i L	V_n L	T °C	V_{nc} L	E_v %	mpe %

Q L/min	V_i L	V_n L	T °C	V_{nc} L	E_v %	mpe %

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Test measures used: _____

β : _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s

Grade: _____

Ambient conditions

Temperature: _____ °C

Humidity: _____ % RH

Pressure: _____ hPa

Remarks:

R 118 was superseded by R 1172:2014

3 Flow interruption

Grade	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	mpe %	E_p Price	MSPD Price
\bar{E}_v	%		\bar{E}_p								

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Test measures used: _____

β : _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s

Grade: _____

Ambient conditions

Temperature: _____ °C

Humidity: _____ % RH

Pressure: _____ hPa

Grade	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	mpe %	E_p Price	MSPD Price
\bar{E}_v	%		\bar{E}_p								

Grade	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	mpe %	E_p Price	MSPD Price
\bar{E}_v	%		\bar{E}_p								

Remarks:

4 Gas elimination device

V_a L	V_i L	V_n L	T °C	V_{nc} L	E_v %	mpe %	$\frac{V_a/V_n}{V_a/V_{nc}}$ %	Air bubble (yes or no)

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Test measures used: _____

β : _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s

Gas meter used: _____

Suction height: _____ m
(for the liquid)

Diameter: _____ mm

Length: _____ m

Ambient conditions

Temperature: _____ °C

Humidity: _____ % RH

Pressure: _____ hPa

Remarks:

R 718 was superseded by R 718-2:2014

5 Variation in the internal volume of hose

X	Y	Y - X	Scale division mL	Variation mL
Mean value of variation mL		Without hose reel		MSVD mL
		With hose reel		2 × MSVD mL

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Model of hose: _____

Length: _____ m

Inner diameter: _____ mm

Maximum operating pressure: _____ MPa

Ambient conditions

Temperature: _____ °C

Humidity: _____ % RH

Pressure: _____ hPa

Remarks:

R 118 was superseded by R 117-2:2014

6 Endurance test (page 1)

Date of accuracy test before endurance test: _____

Liquid: _____

Viscosity: _____ mPa.s

Volume per delivery: _____ L

Total time of endurance test: _____ h

Total volume per meter: _____ L

Resetting between deliveries: Yes/No

Number of stops: _____

Change of grade: Yes/No

Date of accuracy test after endurance test: _____

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Remarks:

R 118 was superseded by R 117-2:2014

6 Endurance test (page 2)

Q() L/min	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	mpe %	E_p Price	MSPD Price
$\bar{E}_v (A) - \bar{E}_v (B)$					%		$\bar{E}_p (A) - \bar{E}_p (B)$				

Q() L/min	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	mpe %	E_p Price	MSPD Price
$\bar{E}_v (A) - \bar{E}_v (B)$					%		$\bar{E}_p (A) - \bar{E}_p (B)$				

Q() L/min	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	mpe %	E_p Price	MSPD Price
$\bar{E}_v (A) - \bar{E}_v (B)$					%		$\bar{E}_p (A) - \bar{E}_p (B)$				

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Test measures used: _____

β : _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s

Grade: _____

Ambient conditions

Temperature: _____ °C

Humidity: _____ % RH

Pressure: _____ hPa

$\bar{E}_v (A)$: Error after endurance test

$\bar{E}_v (B)$: Error before endurance test

Remarks:

7 Dry heat (non-condensing)

Test condition	Q L/min	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	mpe %	E_p Price	MSPD Price
20 °C												
55 °C												
20 °C												

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Remarks:

Note: Normally, this test is carried out in a simulation set-up. However, in the case of test by liquid flow, the following items should be filled in and the tests at each test condition are recommended to be done at least three times.

Test measures used: _____

β : _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s

R 118 was superseded by R 118-2:2014

8 Cold

Test condition	Q L/min	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	mpe %	E_p Price	MSPD Price
20 °C												
- 25 °C												
20 °C												

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Remarks:

Note: Normally, this test is carried out in a simulation set-up. However, in the case of test by liquid flow, the following items should be filled in and the tests at each test condition are recommended to be done at least three times.

Test measures used: _____

β : _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s

R 117-2:2014 was superseded by R 117-2:2014

9 Damp heat, cyclic (condensing)

Test condition	Q L/min	P _u Price/L	H _i %	V _i L	P _i Price	V _n L	T °C	P _c Price	V _{nc} L	E _v %	mpe %	E _p Price	MSPD Price
20 °C 50 % RH													
Damp heat, cyclic (24 hours × 2 cycles)													
20 °C 50 % RH													

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

H_i : Relative humidity indication

Remarks:

Note: Normally, this test is carried out in a simulation set-up. However, in the case of test by liquid flow, the following items should be filled in and the tests at each test condition are recommended to be done at least three times.


Test measures used: _____

β: _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s

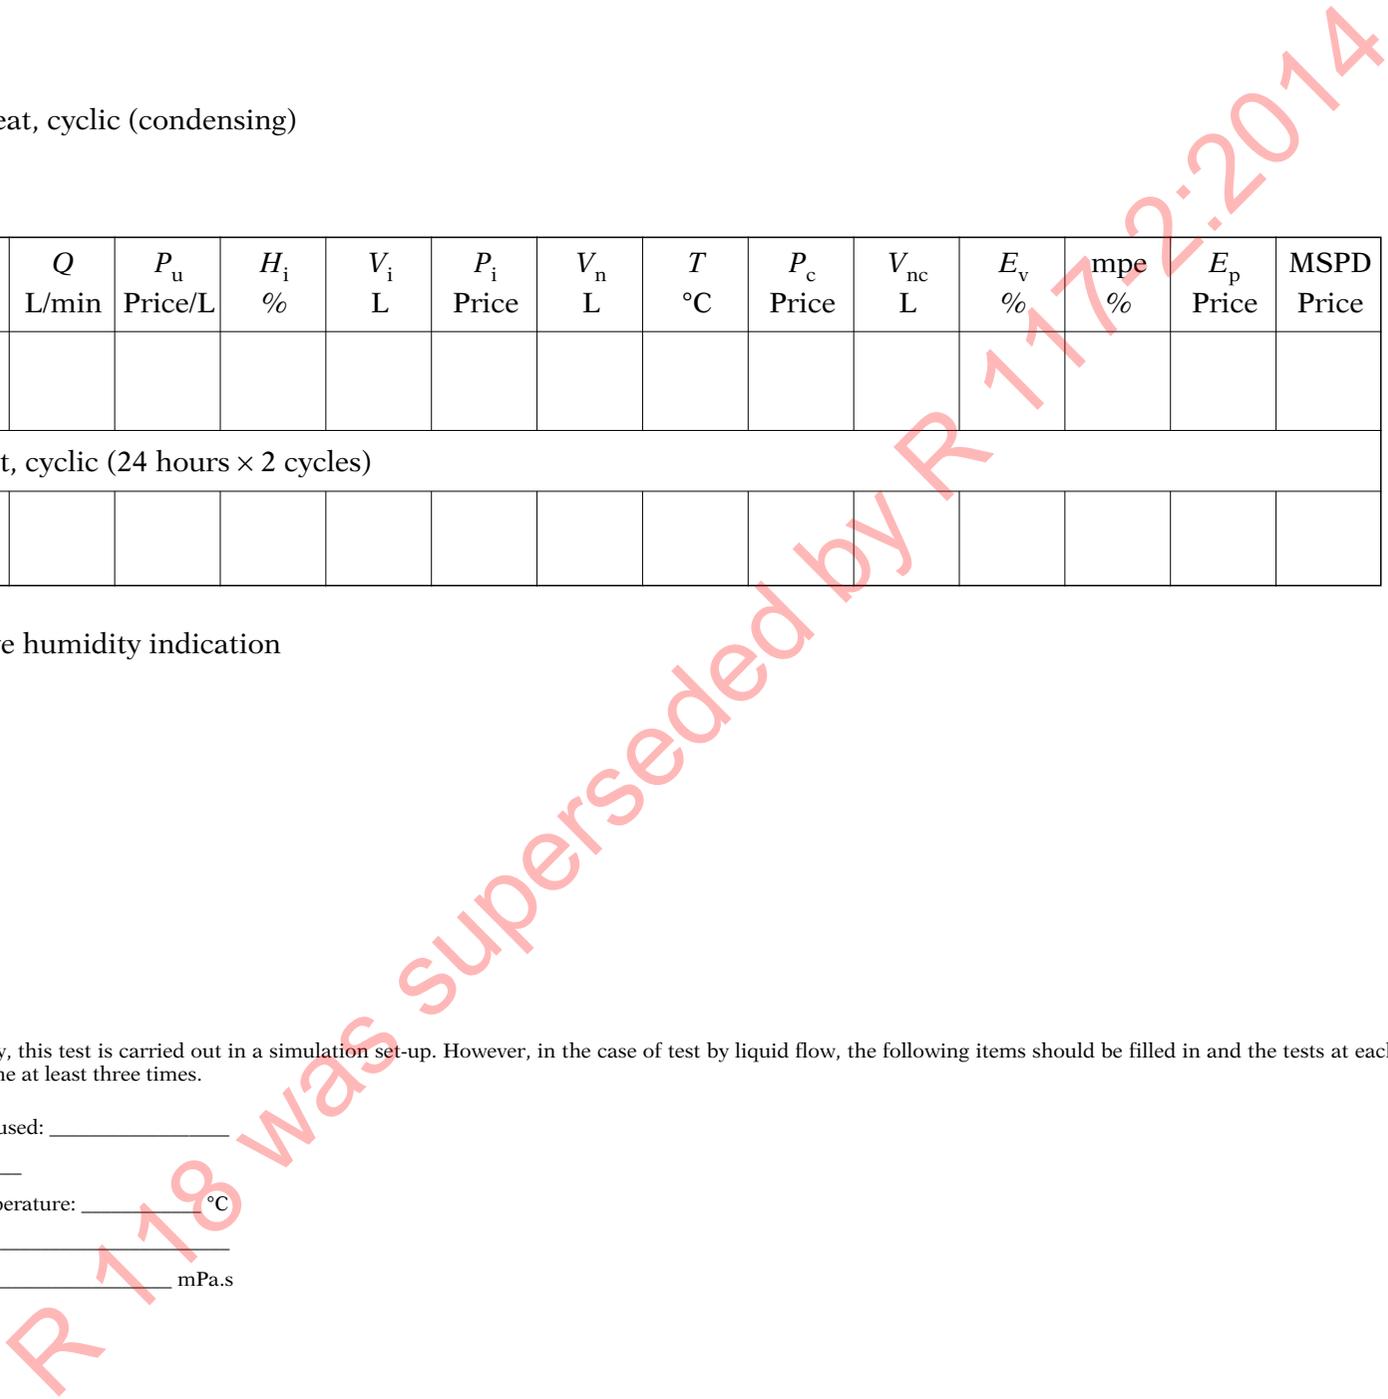

10 Power voltage variation

Test condition	U_i V	Q L/min	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	mpe %	E_p Price	MSPD Price
U													
$1.1 U$													
$0.85 U$													

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

U : Mains voltage

U_i : Indicated mains voltage

Remarks:

- 43 -

Note: Normally, this test is carried out in a simulation set-up. However, in the case of test by liquid flow, the following items should be filled in and the tests at each test condition are recommended to be done at least three times.

Test measures used: _____

β : _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s

R 1178 was superseded by R 1179:2014

11 Short-time power reductions

Test condition	Q L/min	P _u Price/L	V _i L	P _i Price	V _n L	T °C	P _c Price	V _{nc} L	E _v %	S.F. %	E _p Price	MSPD Price	Checking facility	
No reduction													_____	
100 % reduction 1/2 cycle, 10 times													Yes	No
50 % reduction 1 cycle, 10 times													Yes	No

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Remarks:

Note: Normally, this test is carried out in a simulation set-up. However, in the case of test by liquid flow, the following items should be filled in and the tests at each test condition are recommended to be done at least three times.


Test measures used: _____

β: _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s

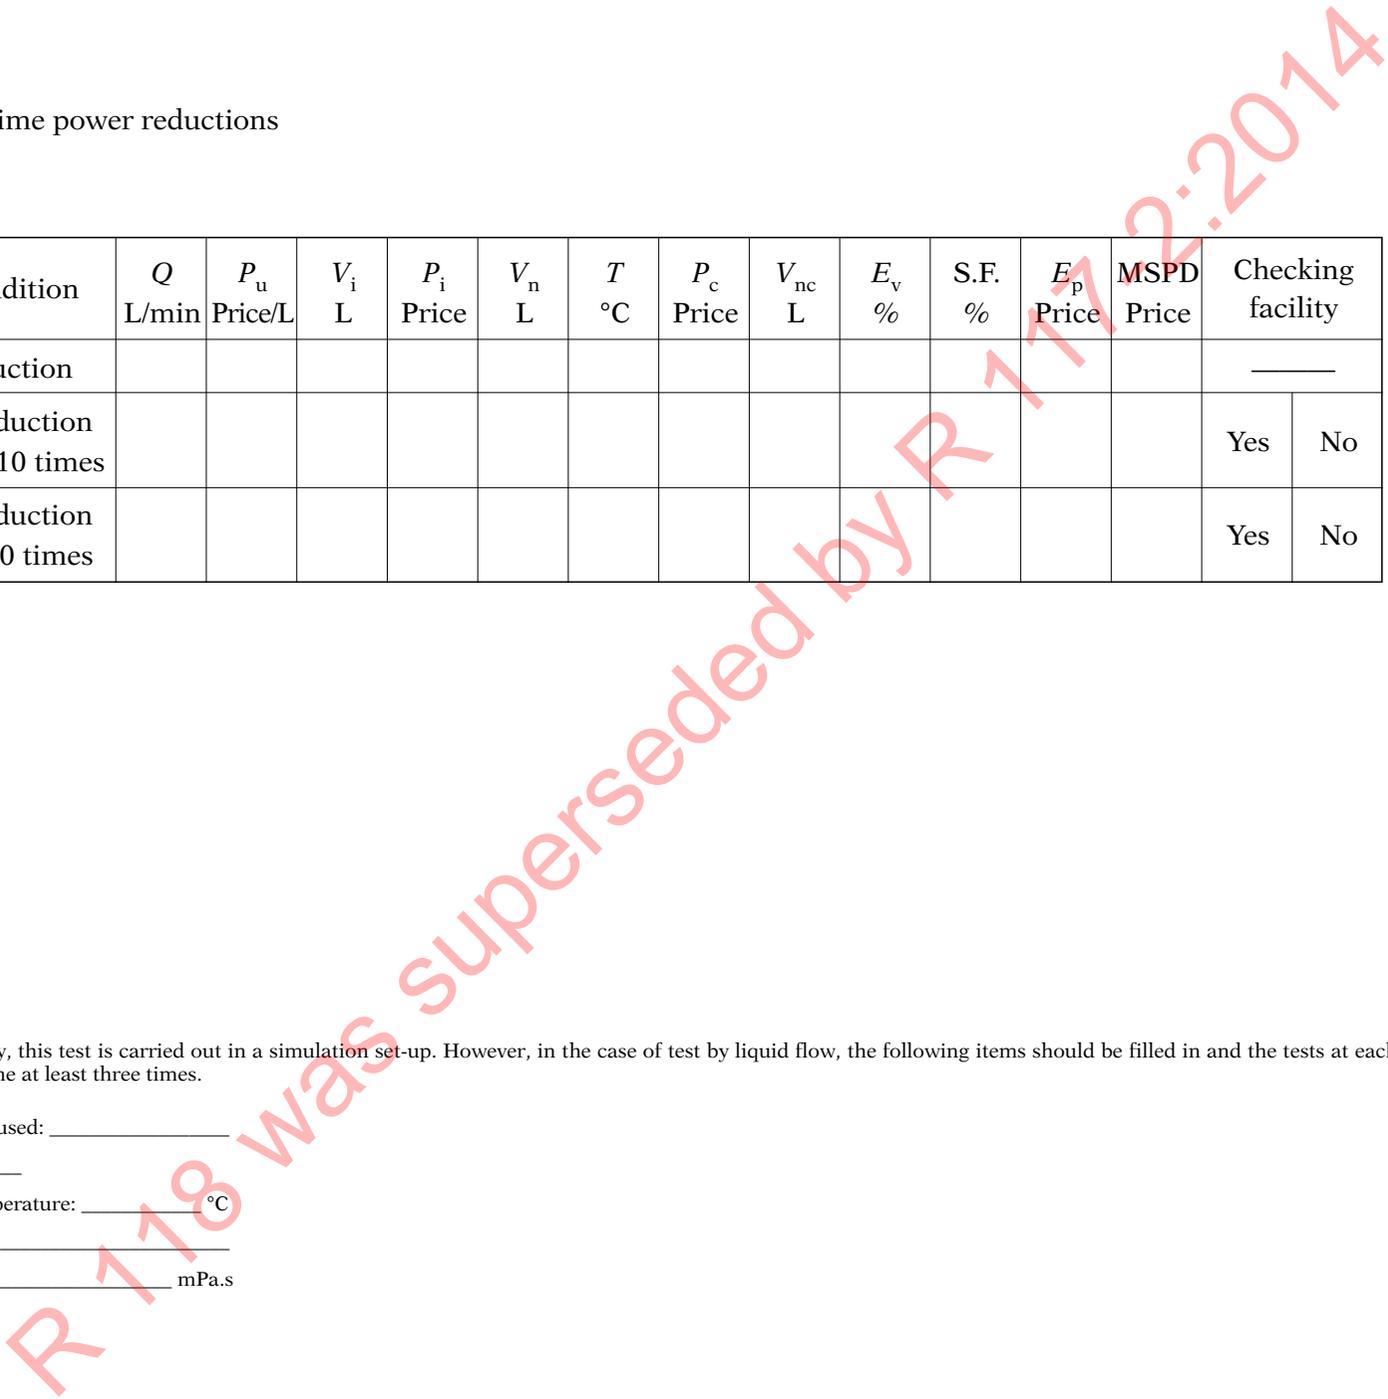

12 Electrical bursts

Test condition	Q L/min	P _u Price/L	V _i L	P _i Price	V _n L	T °C	P _c Price	V _{nc} L	E _v %	S.F. %	E _p Price	MSPD Price	Checking facility	
													Yes	No
Noiseless													_____	
Line 1 Positive													Yes	No
Line 1 Negative													Yes	No
Line 2 Positive													Yes	No
Line 2 Negative													Yes	No

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Line 1 : Phase/Neutral

Line 2 : Phase/Neutral

Remarks:

Note: Normally, this test is carried out in a simulation set-up. However, in the case of test by liquid flow, the following items should be filled in and the tests at each test condition are recommended to be done at least three times.

Test measures used: _____

β: _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s

13 Electrostatic discharges (page 1)

Test condition		Q L/min	P _u Price/L	V _i L	P _i Price	V _n L	T °C	P _c Price	V _{nc} L	E _v %	S.F. %	E _p Price	MSPD Price	Checking facility	
Non-discharge														_____	
Discharged point	C/A													Yes	No
	C/A													Yes	No
	C/A													Yes	No
	C/A													Yes	No
	C/A													Yes	No
	C/A													Yes	No
	C/A													Yes	No

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Ambient conditions

Temperature: _____ °C

Humidity: _____ % RH

Pressure: _____ hPa

C/A: Contact discharge/Air discharge

Remarks:

Note: Normally, this test is carried out in a simulation set-up. However, in the case of test by liquid flow, the following items should be filled in and the tests at each test condition are recommended to be done at least three times.

Test measures used: _____

β: _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s

13 Electrostatic discharges (page 2)

Drawing showing where the discharges have been applied on the surface of the dispenser.

R 118 was superseded by R 117-2:2014

14 Electromagnetic susceptibility

Test condition		S.V. decade/s	Q L/min	P_u Price/L	V_i L	P_i Price	V_n L	T °C	P_c Price	V_{nc} L	E_v %	S.F. %	E_p Price	MSPD Price	Checking facility	
Noiseless															_____	
Antenna method	F.S. 3 V/m 26~500 MHz	V													Yes	No
		H													Yes	No
	F.S. 1 V/m 500~1000 MHz	V													Yes	No
		H													Yes	No
TEM cell method	F.S. 3 V/m 26~500MHz														Yes	No
															Yes	No

Report page ___/___

Application N°: _____

Date: _____

Signature: _____

Ambient conditions

Temperature: _____ °C

Humidity: _____ % RH

Pressure: _____ hPa

S.V.: Sweep Velocity

F.S.: Field Strength

V: Vertical

H: Horizontal

Remarks:

Note: Normally, this test is carried out in a simulation set-up. However, in the case of test by liquid flow, the following items should be filled in and the tests at each test condition are recommended to be done at least three times.

Test measures used: _____

β : _____

Reference temperature: _____ °C

Liquid: _____

Viscosity: _____ mPa.s